



Date :  
 Title : ACCURACY OF MEASURED VS. DERIVED  $\text{S}\bar{\text{V}}\text{O}_2$   
 Authors : H. K. Wallfisch, M.D., Alan S. Tonnesen, M.D.  
 Affiliation: Department of Anesthesia, University of Texas Medical Branch, Galveston, Texas 77550

**Introduction.** Mixed venous  $\text{O}_2$  saturation ( $\text{S}\bar{\text{V}}\text{O}_2$ ) is used to calculate venous  $\text{O}_2$  content ( $\text{C}\bar{\text{V}}\text{O}_2$ ), which is then used to calculate the arterial content to  $\text{C}\bar{\text{V}}\text{O}_2$  difference ( $\text{C}\{\text{a}-\bar{\text{V}}\text{D}\text{O}_2\}$ ), and the pulmonary venous admixture ( $\text{Qva}/\text{Qt}$ ). Mixed venous  $\text{O}_2$  tension ( $\text{P}\bar{\text{V}}\text{O}_2$ ) measurements are often used to calculate  $\text{S}\bar{\text{V}}\text{O}_2$  from formulas, nomograms, or slide rules. The purpose of this study was to assess the accuracy of derived values for  $\text{S}\bar{\text{V}}\text{O}_2$  compared to measured  $\text{S}\bar{\text{V}}\text{O}_2$ , and to evaluate the effect of any discrepancy on subsequent calculations.

**Methods.** Sixty-nine clinically indicated pulmonary artery blood samples were drawn from 19 ICU patients (maximum of 5 drawn from any one patient). Patient temperature, arterial and venous  $\text{PO}_2$ ,  $\text{PCO}_2$ , pH, corrected for patient temperature, and hemoglobin,  $\text{SaO}_2$ , and  $\text{S}\bar{\text{V}}\text{O}_2$  (IL-282 Co-Oximeter) were recorded.  $\text{S}\bar{\text{V}}\text{O}_2$  was then derived from  $\text{P}\bar{\text{V}}\text{O}_2$  using a digital computer subroutine and a standard slide rule. Measured and derived  $\text{S}\bar{\text{V}}\text{O}_2$  values were compared. This study was approved by the institution's Research Committee.

**Results.** Mean measured  $\text{S}\bar{\text{V}}\text{O}_2$  was  $66.6\% \pm 7.9\%$  (range 42.5% - 81%). The mean  $\text{S}\bar{\text{V}}\text{O}_2$  derived from the computer program was  $65.3\% \pm 9.0\%$  (range 43.5% - 85.5%); from the slide rule  $66.5\% \pm 8.1\%$  (range 47% - 82%).

Figure 1 represents the relationship between measured  $\text{S}\bar{\text{V}}\text{O}_2$  and the  $\text{S}\bar{\text{V}}\text{O}_2$  derived from the computer program, and Figure 2, the measured  $\text{S}\bar{\text{V}}\text{O}_2$  and that derived from the slide rule. The solid line on each graph is the line of regression, and the dotted lines bracket the 90% confidence line.

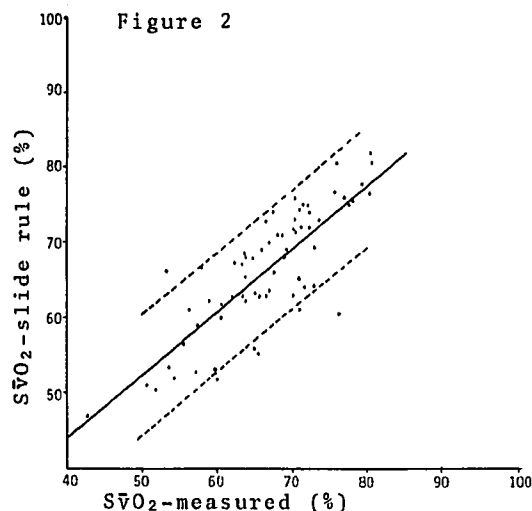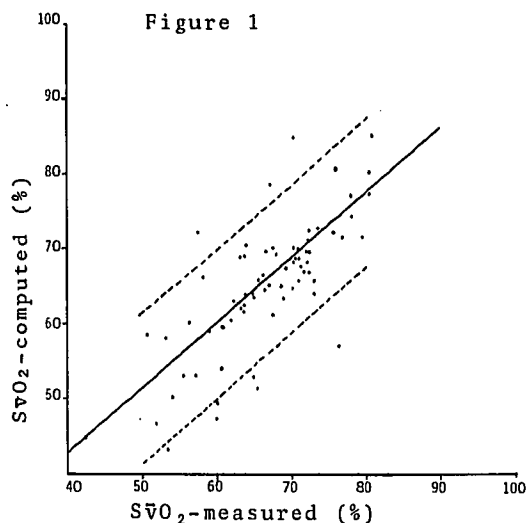

The regression equation for Figure 1 is:  $\text{S}\bar{\text{V}}\text{O}_2\text{-computed} = .87 \times \text{S}\bar{\text{V}}\text{O}_2\text{-measured} + 7.37$ ,  $\text{sy}\cdot\text{x} = 5.83$ ,  $r = .763$  ( $p < .0005$ ). For Figure 2:  $\text{S}\bar{\text{V}}\text{O}_2\text{ slide rule} = .84 \times \text{S}\bar{\text{V}}\text{O}_2\text{-measured} + 10.39$ ,  $\text{sy}\cdot\text{x} = 4.70$ ,  $r = .891$  ( $p < .0005$ ).

Derived  $\text{S}\bar{\text{V}}\text{O}_2$  was used to recalculate  $\text{C}\{\text{a}-\bar{\text{V}}\text{D}\text{O}_2\}$  and  $\text{Qva}/\text{Qt}$  for ten data sets, chosen to span the observed  $\text{Qva}/\text{Qt}$  range. Recalculated  $\text{C}\{\text{a}-\bar{\text{V}}\text{D}\text{O}_2\}$  varied from "true"  $\text{C}\{\text{a}-\bar{\text{V}}\text{D}\text{O}_2\}$  (mean  $4.1 \text{ ccO}_2/\text{dl}$ ) by 0.81 using  $\text{S}\bar{\text{V}}\text{O}_2\text{-computed}$  and by 0.89 using  $\text{S}\bar{\text{V}}\text{O}_2\text{-slide rule}$ . Recalculated  $\text{Qva}/\text{Qt}$  differed from the "true"  $\text{Qva}/\text{Qt}$  (mean .25) by .04 using  $\text{S}\bar{\text{V}}\text{O}_2\text{-computed}$ , and by .05 using  $\text{S}\bar{\text{V}}\text{O}_2\text{-slide rule}$ .

**Discussion.** Using derived  $\text{S}\bar{\text{V}}\text{O}_2$  from the extremes of the 90% confidence interval could result in an error in  $\text{C}\{\text{a}-\bar{\text{V}}\text{D}\text{O}_2\}$  of as much as  $1.9 \text{ ccO}_2/\text{dl}$  (65%), and an error in  $\text{Qva}/\text{Qt}$  of as much as .11 (36%). The above data support our recommendation that accurate evaluation of hemodynamic and pulmonary status of the critically ill patient requires direct measurement of the  $\text{S}\bar{\text{V}}\text{O}_2$ .

#### References

1. Kelman, GR: Digital Computer Subroutine for the Conversion of Oxygen Tension into Saturation. *J Appl Physiol* 21: 1375-1376, 66.
2. Severinghaus, JW: Blood Gas Calculator. *J Appl Physiol* 21: 1108-1116, 66.