

and 04 series patient cable is excellent electrical equipment, which has functioned reliably for us over the last 5 years. As a result, we evolved a policy of replacing reusable electrical equipment only when damage was obvious or suspected. In retrospect, the lack of a regular replacement schedule is what enabled a damaged system to simulate intermittent artifactual S-T segment depression.

Since discovering this problem with apparently undamaged lead wires, we have instituted an informal but

regular replacement schedule for NDM lead wires and patient cables. We offer this information in the hope that other departments will benefit from our experience.

AUGUST M. MANTIA, M.D.
Staff Anesthesiologist
Western Pennsylvania Hospital
4800 Friendship Avenue
Pittsburgh, Pennsylvania 15224

(Accepted for publication September 21, 1984.)

Anesthesiology
62:208-209, 1985

An Unusual Source of Leak in the Anesthesia Circuit

To the Editor:—Equipment-related complications and hazards are well known to the anesthesiologist.¹ Leaks in the anesthesia machine circuit are common occurrences and usually are discovered during a routine machine checkout.^{2,3} Disposable circuits commonly are used and can be the cause of leaks and airway obstruction.⁴⁻⁶ This report illustrates a previously undescribed serious leak in a disposable anesthesia circuit that could not be detected by routine machine check-out.

REPORT OF A CASE

Patient 1, a 16-year-old prima gravida at term underwent emergency cesarean section because of fetal distress. We preoxygenated the patient and induced anesthesia with thiopental and succinylcholine, utilizing a standard rapid-sequence induction. We performed an uneventful laryngoscopy and intubated the trachea with a 7.0-mm endotracheal tube. After inflating the endotracheal tube cuff and

connecting the endotracheal tube to a semiclosed anesthesia circuit, we were unable to ventilate the patient adequately, and there was a significant audible leak. In an attempt to isolate the source of the leak, we independently documented the integrity of the endotracheal tube cuff and the anesthesia circuit. A second attempt at ventilation localized the leak to the plastic elbow of the disposable circuit (fig. 1). We removed the plastic elbow from the circuit and were able to ventilate the patient easily. The infant was delivered with Apgar scores of 7 and 9 at 1 and 5 min, respectively. At the completion of the operation, the patient was extubated awake without problems.

Thorough checkout of the anesthesia machine does not always ensure that leaks significant enough to interfere with ventilation will be detected.⁷ In spite of following a standard protocol that includes pressurizing the breathing system to 40 cm H₂O against a closed relief valve and an occluded patient port,³ we failed to demonstrate a significant hazard. Figure 1 demonstrates a defect in the inner ring of the elbow of a NARDA® nonconductive disposable anesthesia breathing circuit (N1310DN). This leak can be detected if only the inner ring is occluded during the breathing system checkout. This case emphasizes the importance of inspecting as well as testing all anesthesia equipment prior to use.

RICHARD D. COLAVITA, M.D.
Clinical Instructor in Anesthesia

JEFFREY L. APFELBAUM, M.D.
Assistant Professor of Anesthesia

Department of Anesthesia
University of Pennsylvania
School of Medicine
3400 Spruce Street
Philadelphia, Pennsylvania 19104

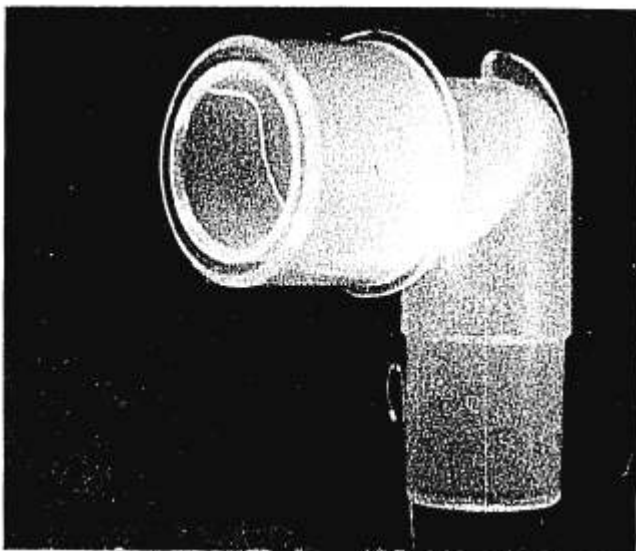


FIG. 1. View of the elbow from the NARDA® disposable anesthesia circuit (N1310DN) demonstrating a defect of the inner ring.

REFERENCES

1. Spooner RB, Kirby RR: Equipment-related anesthesia incidents. *Int Anesthesiol Clin* 92:133-147, 1984

- Mantia AM: A defective Washington T-piece: An example of inevitable failure and lessons to be learned. *ANESTHESIOLOGY* 59:167-168, 1983
- Dorsch JA, Dorsch SE: *Understanding Anesthesia Equipment: Construction, Care, and Complications*, 2nd edition. Baltimore, Williams and Wilkins, 1984, pp 404-405
- Cottrell JE, Bernhard W, Turndorf H: Hazards of disposable rebreathing circuits. *Anesth Analg* 55:743-744, 1976
- Forester AC: Mishaps in anaesthesia. *Anaesthesia* 14:388-399, 1959
- Osterud A: Dangerous fault in disposable connector for oral-tracheal tube. *Br J Anaesth* 46:952, 1974
- Rolbin S: An unusual cause of ventilator leak. *Can Anaesth Soc J* 24:522-524, 1977

(Accepted for publication September 21, 1984.)

Anesthesiology
62:209, 1985

A New Partial Spiral Tube for Nasotracheal Intubation

To the Editor:—Nasotracheal intubation is one of the solutions for both maintenance of an airway and providing an adequate surgical field in oral and maxillo-facial surgery. However, problems still arise with respect to connection of the endotracheal tube to the breathing system. Several types of connectors have been developed for these needs. Although nylon-embedded latex connectors partially can meet these needs,¹ disconnection may still occur, and gas flow resistance is increased due to the internal diameter of the connection part being smaller than that of the endotracheal tube, especially in children. A newly developed connector, FLEXIBEND®, may be one of the best presently available.² An armored latex spiral endotracheal tube has been advocated in an attempt to avoid using connectors in nasotracheal intubation, but obstruction may occur because of its laminated construction.³ In addition, the use of this device is limited in children. Recently, an improved partial spiral endotracheal tube* made of silicon (3.5-9.0 mm ID) has been developed to meet the special needs of oral and maxillo-facial surgery. The distal portion of the tube consists of a conventional curved Magill type tube and the proximal portion of a spiral tube. The length of the two portions of the tube are designed according to the anatomic differences in children and adults (fig. 1). For example, the tube with an 8.0 mm ID consists of Magill type tube of 20 cm length and spiral tube of 16 cm length. When the patient is intubated, the junction of the two portions can be placed inside the nostril. Further, the thickness of the spiral tube is less than that of the Magill type tube so that the tube easily bends at the nostril in any direction for convenient attachment to the breathing system. Blind nasotracheal intubation can also be easily performed. Nasotracheal intubation with this device has proven

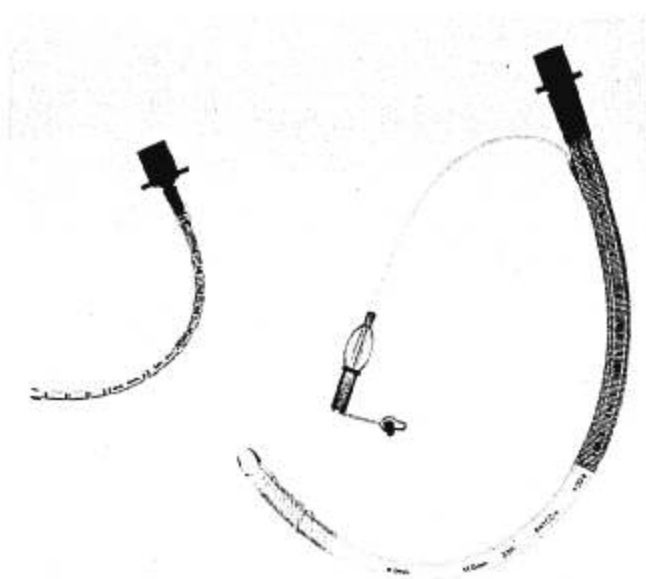


FIG. 1. Partial spiral tubes for children (left) and adults (right).

useful, regardless of the patient's age, for airway management in oral and maxillo-facial surgery in our department.

YOSHIO HATANO, M.D.
TOSHIYUKI ARAI, M.D.
TOKUYA HARIOKA, M.D.
*Department of Anesthesiology
Kyoto University Hospital
Kyoto 606, Japan*

REFERENCES

- Bain JA, Spoerel WE: A nylon embedded latex connector for nasotracheal intubation. *ANESTHESIOLOGY* 60:497-499, 1984
- Shupak RC: A new tracheal tube for head and neck surgery. *ANESTHESIOLOGY* 60:621-622, 1984
- Cohen DD, Dillon JB: Hazards of armored endotracheal tubes. *Anesth Analg* 51:856-858, 1972

(Accepted for publication September 21, 1984.)

* This partial spiral tube named SWAY TUBE® now is produced by Fuji Systems Co., Ltd., 1-11-1, Ebisu, Shibuya-ku, Tokyo 150, Japan.