

REFERENCES

1. Flewellen EH, Nelson TE, Jones WP, Arens JF, Wagner DL: Dantrolene dose response in awake man: Implications for management of malignant hyperthermia. *ANESTHESIOLOGY* 59:275-280, 1983
2. Duncan PG: Availability of dantrolene in Canadian hospitals. *Can Anaesth Soc J* 32:205-209, 1985

3. Rosenberg H: Malignant hyperthermia. *Hosp Pract* 20:139-149, 1985
4. Jantzen JP, Hackett GH, Ellermeyer W, Giesecke AH: Malignant hyperthermia: Successful management of a probable case. *Tex Med* 81:37-42, 1985
5. Britt BA: Another view on central warehousing of dantrolene. *Am J Hosp Pharm* 38:464-467, 1981

(Accepted for publication November 19, 1986.)

Anesthesiology  
66:449, 1987

### A Simpler Tidy Adjunct to Arterial Cannulation

*To the Editor:*—I read with interest the recent letter "A Tidy Adjunct to Arterial Cannulation."<sup>1</sup> I routinely use a similar technique that is even easier.

Provided with each intravenous (or intraarterial) catheter is a transparent plastic shield, designed to protect the needle-catheter assembly during shipment. The shield is hollow, and has a hole in its distal end. Before attempting an arterial puncture, after the plastic plug is removed from the needle, the shield is attached to the proximal end of the needle instead of being discarded (fig. 1). Backflow indicating arterial puncture is then observed inside the shield. From 1-3 cc of backflow can be held in the shield, depending on the type of catheter used.

This technique is equally as "tidy" as the one previously reported. It also is faster and easier to do, and allows you to keep your syringe, already filled with local anesthetic, available for further use.

DONALD S. STEVENS, M.D.  
*Attending Anesthesiologist  
Alachua General Hospital  
Gainesville, Florida 32602*

Anesthesiology  
66:449-450, 1987

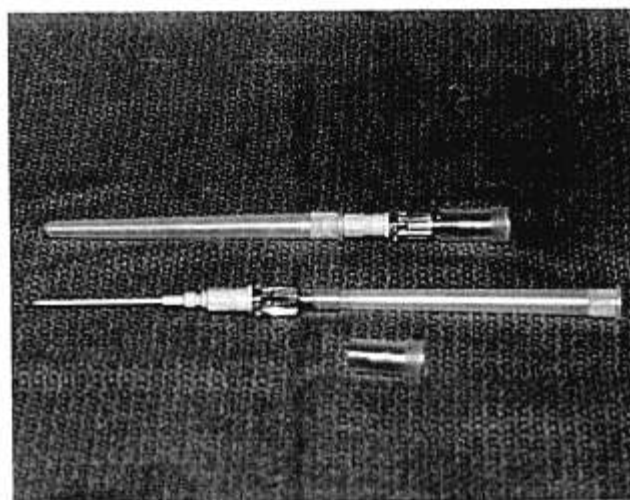


FIG. 1. Catheter and shield before and after re-assembly.

REFERENCE

1. Sabo B, Smith R: A tidy adjunct to arterial cannulation. *ANESTHESIOLOGY* 64:534-535, 1986

(Accepted for publication November 25, 1986.)

### Prevention of Leak of Local Anesthetic from Under a Pneumatic Tourniquet

*To the Editor:*—Grice's<sup>1</sup> investigation of the mechanism of anesthetic leakage under a tourniquet during intravenous regional anesthesia deserves the highest congratulations for clearly defining the source of an occasional life-threatening complication during a generally safe and well-accepted anesthetic technique. One needs only to avoid injecting the local anesthetic at pressures higher than the effective tourniquet pressure. But how can this be done? The authors suggest that injection should be slowed to take at least 90 seconds. This is, however, an indirect way of limiting injection pressure. A much more direct way exists.

DLP Inc. (620 Watson S.W., Grand Rapids, MI 49501-0409) manufactures a "Pressure Sensing Syringe," currently used for distending harvested veins during coronary bypass grafting. This syringe incorporates a tactile feedback sensor which allows the user to avoid exceeding 250 mmHg when distending the vein graft. The company indicates that the syringe can be recalibrated during manufacturing with an upper limit of 170 mmHg, which would allow direct control over the pressure of injection during intravenous regional anesthesia, thereby totally preventing local anesthetic from gaining access to the systemic circulation while the tourniquet is inflated. By using this

syringe, the safety of all intravenous regional anesthesia would be improved, and the recommendations of Ware<sup>2</sup> and Hollingworth *et al.*<sup>3</sup> could be followed with bupivacaine once again becoming the drug of choice for intravenous regional anesthesia.

THEODORE A. NOEL, II, M.D.  
*Staff Anesthesiologist*  
*Florida Hospital*  
*601 E. Rollins*  
*Orlando, Florida 32803*

RICK VAN POPERING  
*Design Engineer*

*DLP Inc.*  
*620 Watson S.W.*  
*Grand Rapids, Michigan 49501*

## REFERENCES

1. Grice SC, Morell RC, Balestrieri FJ, Stump DA, Howard G: Intravenous regional anesthesia: Evaluation and prevention of leakage under the tourniquet. *ANESTHESIOLOGY* 65:316-320, 1986
2. Ware RJ: Intravenous regional anesthesia using bupivacaine. *Anaesthesia* 30:817-822, 1975
3. Hollingworth A, Wallace WA, Dabir R, Ellis SJ, Smith AFM: Comparison of bupivacaine and prilocaine used in Bier block—A double blind trial. *Injury* 13:331-336, 1982

*(Accepted for publication November 20, 1986.)*

**ANNOUNCEMENT**

The American Board of Anesthesiology (ABA) will administer its second written examination in **Critical Care Medicine** on Saturday, September 19, 1987, in Dallas, Texas. Diplomates of the ABA who apply and are judged to be qualified by virtue of their additional training or experience in Critical Care Medicine will be accepted for examination. An application may be requested by writing to the Secretary, American Board of Anesthesiology, 100 Constitution Plaza, Hartford, Connecticut 06103. The deadline for receipt of completed applications in the Board office is June 10, 1987.