

The Non-invasive Determination of Cardiac Output in Children: A Three-breath Technique

William D. Morton, M.D., F.R.C.P.C.*

In this study, the cardiac output of 11 children (5 days to 18 yr of age) was measured following cardiopulmonary bypass. Standard dye dilution cardiac outputs and an indirect Fick-CO₂ technique were simultaneously determined. A rebreathing maneuver is described to estimate the oxygenated mixed venous P_{CO₂} (PvCO₂). This estimate of PvCO₂ was combined with the end tidal P_{CO₂} and CO₂ production to give a non-invasive Fick estimate of the cardiac output. Non-invasive cardiac outputs correlated well with those measured by dye-dilution ($r^2 = 0.94$) over a range of cardiac outputs from 490-7280 ml/min. All non-invasive determinations were within 15% of the line of identity, and within 22% of averaged replicate dye-dilution values. Our results agree with previous comparisons of indirect Fick-CO₂ methods with invasive determinations of cardiac output. These data suggest that the indirect Fick-CO₂ technique offers a rapid, non-invasive alternative to invasive monitoring of cardiac output. (Key words: Anesthesia, pediatrics. Measurement technique, cardiac output: non-invasive.)

IN 1956, COLLIER¹ DESCRIBED a rebreathing technique to estimate the mixed venous P_{CO₂}. Collier's "oxygenated" PvCO₂ is defined as the mixed venous P_{CO₂} measured in the presence of oxygen saturated hemoglobin. With Collier's technique, a patient rebreathes a gas mixture with a CO₂ partial pressure greater than the estimated PvCO₂ to obtain an equilibrium PvCO₂ estimate. Defares² subsequently reported PvCO₂ estimates based on the asymptotic rise in P_{CO₂} during rebreathing. Refinements of the equilibrium and exponential techniques have been used to determine cardiac output by the indirect Fick-CO₂ method.³⁻⁷

Our initial attempts to reproduce stable estimates of PvCO₂ by the equilibrium method were unsuccessful in small (≤ 5.3 kg) subjects. Equilibration of CO₂ could not be obtained within three breaths, inspired and expired gas varied by more than 1 mmHg, and a plateau could not be sustained for 10 s.⁸ On the other hand, these criteria for an adequate equilibrium capnogram were easily replicated in larger subjects.

In this paper, we present a technique to estimate the oxygenated mixed venous P_{CO₂} (PETCO₂) in both large

and small subjects. To reproducibly determine the PvCO₂ in both large and small subjects, we combined a controlled-rebreathing technique described by Fisher,⁹ with an equilibrium rebreathing approach. Our modification allows the inspired P_{CO₂} to equilibrate toward the expired P_{CO₂} during rebreathing. In contrast, Fisher's technique rigidly controls the inspired P_{CO₂}. We calculated cardiac output combining the indirect Fick-CO₂ technique with this estimate of PvCO₂, the end-tidal P_{CO₂} (PETCO₂), and CO₂ production ($\dot{V}CO_2$). These indirect Fick-CO₂ cardiac outputs were compared with simultaneous dye-dilution determinations.

Materials and Methods

The study was approved by the hospital Human Subject Review Committee. We studied 11 patients weighing 2.8-43 kg, aged 5 days-18 yr following elective surgical repair of congenital heart disease. One patient with a residual postoperative left-to-right intracardiac shunt was excluded. All cardiac outputs were measured 1-2 h after patients were transferred to the intensive care unit.

All patients were ventilated by a Siemens 900-C ventilator. We measured $\dot{V}CO_2$ continuously with a Siemens model 930 CO₂ analyzer. This CO₂ analyzer determines $\dot{V}CO_2$ by integrating the product of the instantaneous expiratory flow and the instantaneous expired P_{CO₂}. $\dot{V}CO_2$ was recorded when the $\dot{V}CO_2$ measurement was stable for at least 30 s immediately before the cardiac output determination. Inspiratory and expiratory volumes were compared by a pitot tube flowmeter¹⁰ to assure no endotracheal tube leaks.

A Puritan-Bennett CO₂ analyzer (response time of 200 msec at 150 ml/min flow rate) equipped with a graph recorder was calibrated with dry 5.17% CO₂ before each study. PETCO₂ and all rebreathing CO₂ measurements were sampled from a 19-gauge catheter positioned near the distal tip of the endotracheal tube.

Pulmonary blood flow (PBF) was determined from the Fick equation:

$$PBF(\text{ml}/\text{min}) = \frac{\dot{V}CO_2(\text{ml}CO_2/\text{min})}{CvCO_2 - CaCO_2(\text{ml}CO_2/\text{ml})}$$

where $\dot{V}CO_2$ = production of CO₂, CvCO₂ = CO₂ content of mixed venous blood, and CaCO₂ = CO₂ content of arterial blood. Distal PETCO₂ measurements were used to estimate arterial P_{CO₂} (PaCO₂).¹¹ If arterial

* Lecturer, University of Toronto; Staff Anaesthetist, The Hospital for Sick Children.

Received from the Department of Anesthesia and the Research Institute, The Hospital for Sick Children and University of Toronto, Toronto, Ontario. Accepted for publication March 15, 1988. Supported in part by a grant from the University of Toronto (#3-336-269-50).

Address reprint requests to Dr. Morton: Department of Anaesthesia, St. Joseph's Hospital, 50 Charlton Avenue E., Hamilton, Ontario, Canada L8N 4A6.

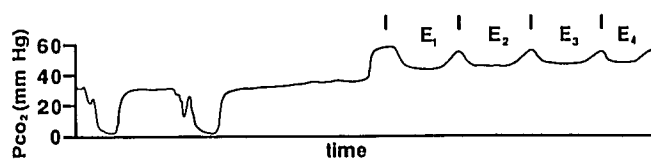


FIG. 1. Capnograph of a single rebreathing maneuver in a 7.2-kg child. $PiCO_2 = 60$ mmHg. The plateau after the third expired breath (E_3) was used to calculate $PvCO_2$ as described in the text. The discontinuity in the ventilated breath at the left of the figure resulted from a brief ventilator disconnection and an attempt at spontaneous ventilation by the patient.

blood gases were not available, a Nellcor® pulse oximeter was used to measure O_2 saturation.

To measure $PvCO_2$, a closed 2-liter reservoir bag was filled from an anesthesia machine equipped with Quantiflex® CO_2 and O_2 flowmeters. The P_{CO_2} of the delivered mixture ($PiCO_2$) was analyzed immediately before the rebreathing maneuver. The endotracheal tube of each patient was disconnected from the ventilator and the patients were allowed to rebreathe for at least four breaths a test gas of 6–9% CO_2 in oxygen. During rebreathing, the ventilator frequency and volume was manually approximated. The expired P_{CO_2} ($PEXCO_2$) following the second, third, and fourth breaths was recorded (fig. 1). This rebreathing maneuver was repeated two to five times with different concentrations of test gas, allowing at least 1 min before repetition. When $PEXCO_2 - PiCO_2$ was plotted as a function of $PiCO_2$, a least-squares linear regression was obtained (fig. 2). The x-intercept ($PEXCO_2 = PiCO_2$) was used as an estimate of $PvCO_2$. This modification of Fisher's technique allows the $PiCO_2$ to equilibrate toward $PvCO_2$ during the rebreathing trial.

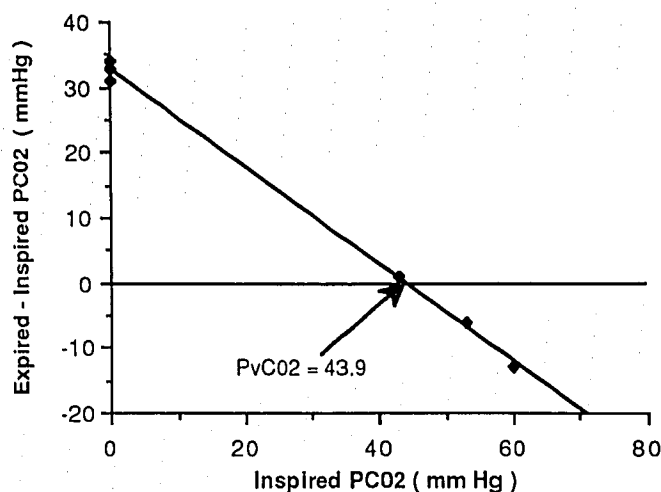


FIG. 2. $PvCO_2$ estimation in a 7.2-kg child. A least-squares regression line is shown. Three separate rebreathing maneuvers produced the three points at the right of the figure. The $PETCO_2$ (where $PiCO_2 = 0$) is shown on the ordinate.

CO_2 contents were calculated from McHardy's¹² mathematical derivation of the CO_2 dissociation curve. Corrections were applied for O_2 saturation and hemoglobin concentration.

$$CvCO_2 - CaCO_2 = 11.02(PvCO_2^{0.996} - PaCO_2^{0.996})$$

$$- 0.015(PvCO_2 - PaCO_2)(15 - Hb)$$

$$- 0.064(95 - SaO_2),$$

where $CvCO_2 - CaCO_2$ is the mixed venous-arterial CO_2 content difference in ml of $CO_2/100$ ml of blood, $PvCO_2$ is the oxygenated mixed venous tension of CO_2 in mmHg, $PaCO_2$ is approximated by $PETCO_2$, SaO_2 is the percent O_2 saturation of arterial blood, and Hb is the hemoglobin concentration in gm/100 ml blood.

Dye dilution cardiac outputs were determined immediately after the indirect-Fick cardiac outputs. Cardio-green dye (1.25–5.0 mg) was rapidly injected into a superior vena caval catheter or left atrial catheter at end-exhalation. A Waters COR-10 cardiac output computer continuously analyzed arterial blood and integrated the resultant dye-dilution curves. Indirect Fick- CO_2 cardiac outputs and dye-dilution outputs were compared by linear regression analysis.

In a parallel study, the oxygenated $PvCO_2$ was determined in 12 subjects (2.8–84 kg) using both the equilibrium technique⁸ and our three-breath method.

Results

Table 1 shows the demographic profile of our patients, including indirect-Fick and dye-dilution cardiac output determinations. The two-, three-, and four-breath cardiac outputs were calculated from the $PvCO_2 - PETCO_2$ gradient as described using $PEXCO_2$ after the second, third, and fourth breath.

The correlation between two-, three-, and four-breath Fick cardiac outputs and dye-dilution cardiac outputs was best using the three-breath maneuver ($r^2 = 0.87, 0.94, \text{ and } 0.90$, respectively). Figure 3 shows the concordance plot of three-breath Fick- CO_2 cardiac outputs with simultaneous dye-dilution determinations. All Fick outputs were within 22% of the averaged dye-dilution values.

We found the three-breath technique gave estimates of $PvCO_2$ 2–4 mmHg lower than the equilibrium method. Figure 4 shows the correlation between the three-breath $PvCO_2$ determination and the equilibrium values ($r^2 = 0.91$) in 12 subjects. The difference between the two estimates of $PvCO_2$ did not vary with weight ($r^2 = 0.29$). Seven patients in the cardiac output study had rebreathing capnograms with a plateau allowing equilibrium estimates of $PvCO_2$. The mean equilibrium—three-breath $PvCO_2$ difference was 3.93 ± 1.51 mmHg ($\pm SD$) in this group.

TABLE 1. Demographic and Cardiac Output Data

Patient	Weight (kg)	Age	Lesion	vCO ₂ (ml CO ₂ /min)		Hb (g/l)	Oxygen Saturation (%)	Number of Re-breathing Replicates	Calculated Cardiac Output (ml/min) After 'n' Expired Breaths			Mean Dye-dilution Cardiac Output (ml/min) (n = 3)
				(ml/min)	(ml/kg/min)				n = 2	n = 3	n = 4	
A	7.17	8 months	VSD	59	8.2	152	100	3	1130	1030	940	1270
B (Day 1)	12.6	3.5 yr	Tetralogy of Fallot	86	6.8	115	98.8	2	3490	2530	2340	2030
B (Day 2)				96	7.6	103	100	2	2110	2060	1420	2000
C	39.4	14 yr	Aortic aneurysm	190	4.8	110	100	2	6070	5640	5020	7280
D	2.8	5 days	Transposition of great arteries	24	8.6	100	90	3	420	380	350	490
E	34.1	9 yr	VSD	205	6.0	125	100	2	5720	4660	4440	4350
F	43.3	18 yr	Glenn shunt-defect (tetralogy repaired in past)	230	5.3	139	82	5	7750	6430	5820	6340
G	13.4	3.5 yr	AVSD	74	5.5	98	100	2	2110	1920	1690	1680
H	35.4	13 yr	Tetralogy of Fallot	205	5.8	120	100	2	4980	4220	3900	3900
I	10.7	1 month	ASD Type I	94	8.8	135	100	2	2180	2060	1910	1730
J	19.9	5 yr	ASD	123	6.2	103	100	3	3660	3080	2810	2480

Discussion

We describe a rapid, practical method to non-invasively determine cardiac output of small subjects. Previously described non-invasive Fick techniques rely on one of two methods to estimate PvCO₂: 1) the equilibrium method of Collier as refined by McEnvoy *et al.*,⁸ and 2) exponential methods. In infants, rapid CO₂ recirculation yields a rebreathing capnograph that does not rise to an asymptotic value of PvCO₂; despite altering rebreathing bag volumes, a continuous rising P_{CO2} with persistent ventilatory oscillations is seen.

To estimate cardiac output using the three-breath determination of PvCO₂ described, arterial blood samples are not required. Although the blood-gas equilibrium

of alveolar CO₂ is a contentious issue,¹³ at rest the normal PETCO₂-PaCO₂ gradient has been measured to be -2.5 mmHg.⁸ We found a similar gradient (-2 to -4 mmHg) between the three-breath estimate of PvCO₂ and the equilibrium estimate in our study. The Fick cardiac outputs based on the equilibrium PvCO₂-PaCO₂ gradient should, therefore, be expected to be similar to those based on a three-breath PRBCO₂-PETCO₂ gradient.

As pulmonary dead space increases, the Collier estimate of PvCO₂ is not affected, since alveolar, end-tidal, and dead space gas should be in equilibrium. If dead space is increased, a large PETCO₂-PaCO₂ gradient and, therefore, an artifactually low cardiac output will result if the PvCO₂-PETCO₂ gradient is calculated using the

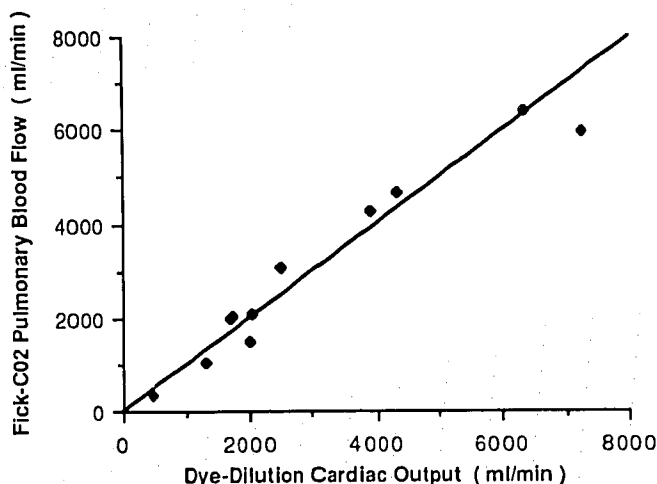


FIG. 3. A concordance plot showing the correlation between non-invasive Fick and dye-dilution determinations of cardiac outputs ($r^2 = 0.94$). The line of identity is shown.

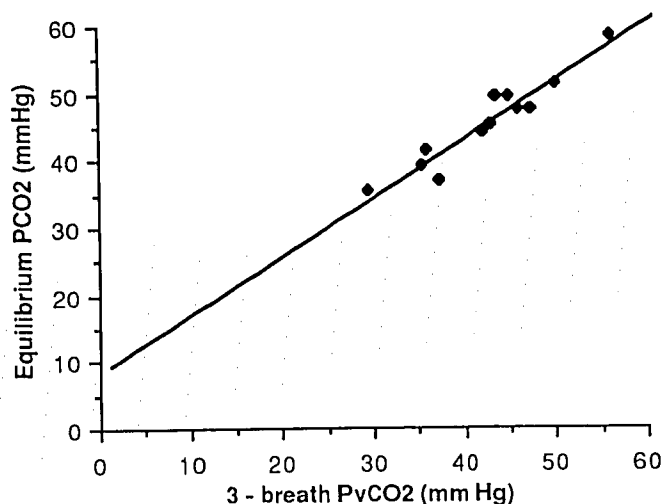


FIG. 4. Least squares regression plot of PvCO₂ as determined by the equilibrium and three-breath technique ($r^2 = 0.91$). The regression line is represented by the curve $y = 0.886x + 8.039$.

equilibrium method.¹⁴ The concordance of our Fick- CO_2 and dye dilution cardiac outputs indicates that the three-breath PRBCO_2 - PETCO_2 gradient accurately reflects the PvCO_2 - PaCO_2 gradient. We speculate that the same factors that lead to an increased PETCO_2 - PaCO_2 gradient also increase the three-breath PRBCO_2 - PvCO_2 gradient, and yield accurate pulmonary blood flow determinations.

If this assertion is correct, we would expect that the three-breath technique will estimate the effective pulmonary blood flow (which will ordinarily equal the systemic cardiac output), will be resistant to error resulting from increased dead space (for example, rapid shallow respirations), and will underestimate the actual pulmonary blood flow in states with increased venous admixture (pulmonary hypotension or pulmonary embolism). Our finding that PBF can be rapidly, non-invasively estimated within 22% of dye-dilution methods suggests that this technique will be clinically useful.

The author gratefully acknowledges the assistance of Ms. Shue Lin Loo in the preparation of this manuscript.

References

1. Collier CR: Determination of mixed venous CO_2 tensions by re-breathing. *J Appl Physiol* 9:25-29, 1956
2. Defares JG: Determination of PvCO_2 from the exponential CO_2 rise during re-breathing. *J Appl Physiol* 13:159-164, 1958
3. Defares JG, Wise ME, Duyaff JW: New indirect Fick procedure for the determination of cardiac output. *Nature* 192:760-761, 1961
4. Muiresan G, Sorbini CA, Solinas E, Grassi V, Casucci G, Petz E: Comparison of CO_2 -rebreathing and direct Fick methods for determining cardiac output. *J Appl Physiol* 24:424-429, 1968
5. Farhi LE, Nesarajah MS, Olszowka AJ, Metildi LA, Ellis AK: Cardiac output determination by simple one-step re-breathing technique. *Respir Physiol* 28:141-159, 1976
6. Davis CC, Jones NL, Sealey BJ: Measurements of cardiac output in seriously ill patients using a CO_2 re-breathing method. *Chest* 73:167-172, 1978
7. Roy RJ, Capek J: Noninvasive cardiac output monitoring using partial CO_2 re-breathing (abstract). *ANESTHESIOLOGY* 63:A172, 1985
8. McEvoy JDS, Jones NC, Campbell EJM: The mixed venous and arterial pCO_2 . *Br Med J* 4:687-690, 1974
9. Fisher JA, Ansel C: A new approach to non-invasive oxygenated mixed venous PCO_2 (abstract). *Clin Invest Med* 9:A24, 1986
10. Wolf AR, Volgyesi GA: A modified Pitot tube for the accurate measurement of tidal volume in children. *ANESTHESIOLOGY* 67:775-778, 1988
11. Badgwell, JM, Heavner JE, May WS, Goldthorn JF, Lerman J: End-tidal P_{CO_2} monitoring in infants and children ventilated with either a partial re-breathing or a non-re-breathing circuit. *ANESTHESIOLOGY* 66:405-410, 1987
12. McHardy GJR: Relationship between the difference in pressure and content of carbon dioxide in arterial and venous blood. *Clin Sci* 32:299-309, 1967
13. Piiper J: Blood-gas equilibrium of carbon dioxide in lungs: A continuing controversy. *J Appl Physiol* 60:1-8, 1986
14. Mahler DA, Matthay RA, Snyder PE, Neff Rk, Loke J: Determination of cardiac output at rest and during exercise by carbon dioxide re-breathing method in obstructive airway disease. *Am Rev Respir Dis* 131:73-78, 1985