

Comparison of the LMA-Classic™ with the New Disposable Soft Seal Laryngeal Mask in Spontaneously Breathing Adult Patients

André A. J. van Zundert, M.D., Ph.D.,* Kristine Fonck, M.D.,† Baha Al-Shaikh, F.F.A.R.S.C.I.,‡ Eric Mortier, M.D., Ph.D.§

Background: The laryngeal mask airway *LMA-Classic*™ has been used widely in clinical practice. A new disposable supra-glottic airway device, the Soft Seal LM, has been introduced recently. In a randomized study, the authors compared the *LMA-Classic*™ and the disposable Soft Seal LM in terms of their clinical performance, cuff pressures during nitrous oxide anesthesia, position of the laryngeal mask *in situ* by fiberoptic evaluation, and morbidity in a wide range of routine general surgery procedures.

Methods: A total of 200 adult patients were randomly assigned to a size 4 laryngeal mask in two equal-sized groups for airway management during surgery: (1) *LMA-Classic*™ (Intavent Orthofix Ltd., Maidenhead, Berkshire, United Kingdom); or (2) Soft Seal LM (Portex Ltd., Hythe, Kent, United Kingdom). Anesthesia was administered with fentanyl, propofol, nitrous oxide, oxygen, and sevoflurane. The variables studied were ease of insertion, fiberoptic view, time *in situ*, incidence of blood on the laryngeal mask at the time of removal, and the incidence of postoperative sore throat at 2 and 24 h. The laryngeal mask cuff pressures were measured continuously. Intracuff pressure limitation was not attempted.

Results: The *LMA-Classic*™ and the Soft Seal LM showed similar clinical performances, as shown by their insertion time (successful insertion at first attempt was achieved within 20 s in 97% with *LMA-Classic*™ vs. 95% with Soft Seal LM), fiberoptic evaluation of the anatomic position of the laryngeal mask, and satisfactory anesthesia conditions. Laryngeal mask cuff pressures increased from 45 to 100.3 mmHg in the *LMA-Classic*™ and from 45 to 46.8 mmHg in the Soft Seal LM ($P < 0.001$). Macroscopic blood was seen on only four occasions in the *LMA-Classic*™ group. The incidence of sore throat was significantly increased at 2 h postoperatively when using the *LMA-Classic*™, although there was no difference at 24 h after surgery.

Conclusions: In spontaneously breathing adult patients requiring a size 4 laryngeal mask airway, the new disposable Soft Seal LM device is an acceptable alternative to the reusable *LMA-Classic*™, resulting in a good laryngeal seal and offering similar clinical performance. Cuff pressures increase substantially when the *LMA-Classic*™ is used but not when using the Soft Seal LM. There was less trauma to patients using the Soft Seal LM, as assessed by the incidence of sore throat in the early postoperative period.

* Professor of Anesthesiology, Department of Anesthesiology, Intensive Care and Pain Therapy, Catharina Hospital. † Staff Anesthesiologist, § Professor of Anesthesiology, Department of Anesthesiology, University Hospital. ‡ Consultant Anaesthetist and Honorary Senior Lecturer, The William Harvey Hospital.

Received from the Department of Anesthesiology, Intensive Care and Pain Therapy, Catharina Hospital, Eindhoven, The Netherlands; the Department of Anesthesiology, University Hospital, Ghent, Belgium; and The William Harvey Hospital, Ashford, Kent, United Kingdom. Submitted for publication December 19, 2002. Accepted for publication June 10, 2003. Supported by The Catharina Foundation, Eindhoven, The Netherlands, and Portex Ltd., Hythe, Kent, United Kingdom, who provided the study samples.

Address correspondence to Dr. van Zundert: Department of Anesthesiology, Intensive Care and Pain Therapy, Catharina Hospital, Michelangelolaan 2, NL-5623 EJ Eindhoven, The Netherlands. Address electronic mail to: zundert@iae.nl. Individual article reprints may be purchased through the Journal Web site, www.anesthesiology.org.

THE reusable laryngeal mask airway (*LMA-Classic*™, Intavent Orthofix Ltd., Maidenhead, Berkshire, United Kingdom) has been available since 1988, and it is now widely used for airway management during elective general anesthesia not requiring tracheal intubation. A single-use laryngeal mask airway (*LMA-Unique*™, Intavent Orthofix Ltd.) has been available since 1997, and it has been found to be similar in performance to the reusable laryngeal mask.¹⁻⁴ There is growing concern regarding the ability to clean reusable laryngeal masks effectively and consequently their safety.⁵⁻¹⁰

A new single-use disposable supra-glottic airway device, the Soft Seal LM (Portex Ltd., Hythe Kent, United Kingdom), has been introduced recently (fig. 1). It is fabricated from latex-free medical-grade plasticized polyvinyl chloride (PVC). To our knowledge, no studies have been published so far assessing this device. The characteristics of the two laryngeal masks are presented in table 1.

The primary aim of this study was to evaluate the clinical acceptability of the new device, the Soft Seal LM, as an alternative to the *LMA-Classic*™. We compared the masks in terms of ease of insertion, cuff pressure changes, position *in situ* by fiberoptic evaluation, and morbidity.

Materials and Methods

After institutional review board approval (Catharina Hospital Eindhoven) and informed patient consent, we prospectively studied 200 unselected, consecutive, supine anesthetized patients who were scheduled to undergo elective surgery with the use of a laryngeal mask. Patients aged 18-80 yr were included in the study. Patients were excluded if they had an American Society of Anesthesiologists physical status class of III to V; required surgery in a nonsupine position or had to undergo oral or nasal surgery; had a preoperative sore throat; had a known or predicted difficult airway, chronic obstructive pulmonary disease, or respiratory tract pathology; or were considered unsuitable for surgery with the use of a laryngeal mask.

Patients were allocated randomly, using computer-generated tables of random numbers, to a size 4 laryngeal mask and received either the silicone rubber reusable *LMA-Classic*™ or the disposable Portex Soft Seal LM. All laryngeal masks were inserted for a wide range of routine general surgery, orthopedic, urologic, gynecologic, and plastic surgery. Patients were unaware of the airway

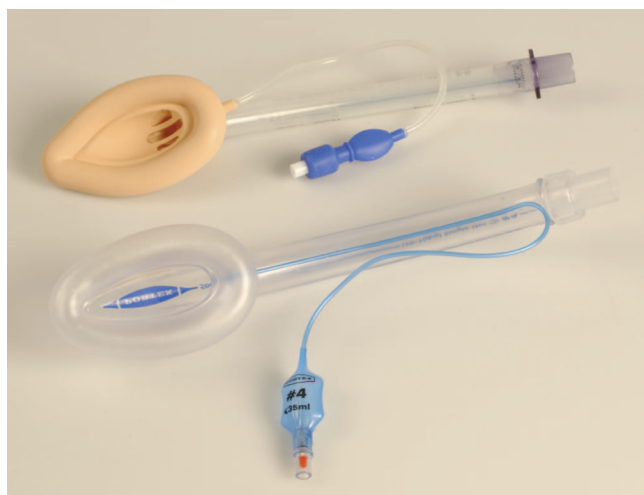


Fig. 1. The reusable *LMA-Classic™* and the disposable Soft Seal LM. Note the same dimensions of the cuff, whereas the diameter of the tube and the depth of the bowl are larger in the disposable laryngeal mask. The inflation line is integrated in the disposable version while separate in the *LMA-Classic™*. Two laryngeal bars are present in the *LMA-Classic™* but absent in the disposable Soft Seal LM. Note the size of the product and maximum cuff inflation volume (< 35 ml) printed on the pilot balloon of the Soft Seal LM.

device used. The *LMA-Classic™* masks used were normal clinical-use products in our hospital. The Soft Seal LMs were all new, as they were used only once. At our institution, the *LMA-Classic™* is the standard supraglottic airway device. All laryngeal masks in both groups were inserted by the same anaesthesiologist (A. V. Z.; personal experience: more than 2,500 *LMA-Classic™* masks and 80 Soft Seal LMs inserted before the study).

Routine preinsertion tests of the cuff for leaks, as recommended by the manufacturers, were done immediately before use. The tip of the laryngeal mask as well as the posterior aspect of the mask was coated with a water-soluble lubricant with 2% lidocaine (Instillagel; Farco-Pharma, Cologne, Germany), which is the normal practice in our institution. The cuff was inflated before insertion with ambient room air at 10 mmHg (15 cm H₂O) above atmospheric pressure, which is the standard practice in our institution and advocated by many authors.^{3,11–18}

No premedication was used, and all patients were preoxygenated for 3 min before intravenous induction. Intravenous induction of general anesthesia consisted of 1 µg/kg fentanyl and 3 mg/kg propofol. The lungs were ventilated manually with sevoflurane (end-tidal 2%–3%) added to a mixture of 66% N₂O in oxygen administered *via* a facemask without the use of an oral airway. The laryngeal mask was inserted 1 min after completion of induction and after loss of lash reflex and the relaxation of the jaw.¹⁹ An insertion attempt was defined as placement of the laryngeal mask in the mouth and withdrawal of the device from the mouth. Successful placement of an effective airway and adequate ventilation was confirmed by the presence of resistance to further downward movement, observing chest wall movement with manual ventilation, listening to the escape of gas from the mouth, detection of a square wave trace capnograph during manually assisted ventilation, and observation of movement of the reservoir bag on spontaneous ventilation. The ease of insertion of the laryngeal mask was

Table 1. Characteristics of Reusable *LMA-Classic™* and Disposable Soft Seal LM, Size 4

	Reusable <i>LMA-Classic™</i>	Disposable Soft Seal LM
Material	Silicone rubber Silicone rubber cuff Translucent–opaque tube Two pieces “Step” between tube and shoe	Medical grade PVC Soft Seal PVC cuff Translucent tube Smooth one-piece device No “step” between tube and shoe
Inflation line	Separate–on cuff Can become tangled with other lines and teeth	Integrated with tube Attached close to 15-mm connector
Marking	Black line	Blue line
Dimensions		
Cuff	90 × 55 mm	90 × 55 mm
Tube	11.0 mm ID 16.0 mm OD	11.0 mm (internal) 17.6 mm (external)
Volume tube	20 ml	33.5 ml
Epiglottis bars	Two	None
Insertion of ETT (<i>in vitro</i>)	Up to 6.0 mm	Up to 7.0 mm
Use of flexible fiber-optic device through LM	Easy to use	Easy to use
Cost		
Device acquisition	140 €	10–12 €
Sterilization/cleaning	2.72 €	Not applicable
Removal of LM	Requires immersion in water to prevent encrustation of residues Requires expensive time-consuming cleaning, washing, and sterilizing	Hospital clinical waste system

ETT = endotracheal tube; LM = laryngeal mask; PVC = polyvinyl chloride.

graded as (1) very easy insertion at the first attempt with no resistance; (2) easy insertion at the first attempt with little resistance; (3) some difficulties, but successful at the second attempt; or (4) not successful.

When the black line (*LMA-Classic*TM) or blue line (Soft Seal LM) was centrally positioned, the laryngeal mask pilot balloon cuff pressure was adjusted to 45 mmHg (60 cm H₂O) as recommended,²⁰⁻²⁴ using a hand-held pressure gauge to monitor the initial cuff pressure in cm H₂O (Endotest; Rüsch, Kern, Germany) and a pressure transducer (AS/3; Datex-Ohmeda, Helsinki, Finland) to measure the cuff pressure continuously in mmHg. The laryngeal mask was securely fixed using tape with a bite block. Subsequently, the seal around the larynx by the laryngeal mask was checked for any air leak by ventilating the patient against an outlet valve pressure of 15 mmHg (20 cm H₂O).²⁵ For that reason, we closed the expiratory valve of the circle system at a fixed gas flow of 3 l/min and noted the airway pressure at which equilibrium was reached. Any air entering the stomach was noted when measuring oropharyngeal leak pressure by listening over the epigastrium with a stethoscope. When the laryngeal mask was considered to function adequately, allowing the patient to breathe spontaneously (sevoflurane-nitrous oxide-oxygen) with end-tidal carbon dioxide levels between 4.0 and 6.0, a fiberoptic (StyletScope; Nihon Kohden, Tokyo, Japan) was inserted with its tip located at the inner aperture of the laryngeal mask. The position of the epiglottis was assessed using a standardized²⁵⁻²⁶ four-point scale (1-4) as follows: grade 4, only vocal cords seen; grade 3, vocal cords and posterior epiglottis seen; grade 2, vocal cords and anterior epiglottis seen; grade 1, vocal cords not seen. Grade 3 and 4 positions were considered correct, whereas grades 1 and 2 were considered suboptimal positions.²⁵ All fiberoptic scoring was made within approximately 2 min of the laryngeal mask insertion. The presence of any aspirated or regurgitated material in the hypopharynx and the incidence of laryngeal spasm or other adverse events (coughing, retching, breath holding) were noted.

Anesthesia was maintained with a fresh gas flow of 3 l/min using 66% N₂O in oxygen and sevoflurane (end-tidal sevoflurane levels between 1.5% and 2%). Fentanyl, 0.05 mg, was added intravenously as required. When surgically indicated, but well after the insertion of the laryngeal mask airway and fiberoptic score, 0.5 mg/kg rocuronium was used as the neuromuscular blocking drug. Standard patient monitoring consisted of inspiratory and expiratory concentrations of nitrous oxide, oxygen, and sevoflurane; electrocardiogram; heart rate; capnography; noninvasive arterial blood pressure; peripheral oxygen saturation measured by pulse oximetry; respiratory rate; and tidal volume.

At the end of surgery, nitrous oxide and sevoflurane were discontinued to allow the patient to resume full recovery. When the protective reflexes had returned to

normal, the laryngeal mask was removed synchronously with deflation of the cuff to 45 mmHg (60 cm H₂O) to avoid secretions entering the larynx or provoking laryngeal spasms.²¹ On removal of the laryngeal mask, the presence or absence of blood was noted. Any blood on the mask or in the secretions on the mask was considered positive. Patients were requested to grade any sore throat at 2 and 24 h after surgery. Postoperative evaluations, including the evaluation of blood on the laryngeal mask, were performed by another anesthesiologist.

The following parameters of each patient were collected: sex, age, weight, height, type of surgery, time to insert the laryngeal mask, number of insertion attempts to achieve a satisfactory airway, and duration of laryngeal mask *in situ*. Laryngeal mask cuff pressures were monitored continuously, while intracuff pressure limitation was not practiced, with time 0 the moment the pilot cuff was inflated to a pressure of 45 mmHg until the moment nitrous oxide was switched off.

Statistical Analysis

We estimated the final cuff pressure difference between the *LMA-Classic*TM and the Soft Seal LM to be 35% lower in the latter. Sample size calculation was performed using Sampsize version 2.0 (Sample Size tables for clinical studies; Blackwell Science Ltd., Oxford, United Kingdom). Ho: $\mu_1 = \mu_2$ (no difference between population means, two-sided hypothesis). The study had a power of 90% ($\beta = 10\%$; $\alpha = 0.05$), and the standardized difference was 0.35 (SD, 0.86). The estimated sample size was 88 patients per group. Two groups of 100 patients were chosen. Statistical analysis was performed using SPSS version 9.0 for Windows (SPSS Inc., Chicago, IL). Mann-Whitney U and Kruskal-Wallis nonparametric data analyses were used for analysis of variables accordingly in addition to the chi-square test. All data are presented as mean \pm SD. Statistical significance was considered at $P < 0.05$.

Results

The two studied groups were similar in age, sex, weight, and height (table 2). Facemask ventilation before the laryngeal mask insertion in all patients was easy, and no patient needed an oral airway to maintain the airway. In two patients (one in each group), a continuous leak of the airway existed because a good seal could not be obtained, and intubation was chosen. Data from these patients have been excluded, and the cases were repeated. In all other patients, adequate insertion of the laryngeal mask was obtained. The overall laryngeal mask insertion time was within 20 s and successful on the first insertion attempt in 97% of the *LMA-Classic*TM group and 95% of the Soft Seal LM group (table 2). In 3% of the *LMA-Classic*TM group and 5% of the Soft Seal LM group,

Table 2. Demographic and Overall Patient Data

	<i>LMA-Classic</i> TM (n = 100)	Soft Seal LM (n = 100)	P Value*
Male:female ratio	29:71	28:72	NS
Age, yr	46.3 ± 16.3	44.4 ± 16.4	NS
Weight, kg	70.8 ± 9.1	68.3 ± 9.5	NS
Height, cm	167.7 ± 8.4	165.3 ± 6.1	NS
Duration of anesthesia, min	59.6 ± 27.9	61.5 ± 32.5	NS
Minimum–maximum, min	20–140	20–140	NS
Ease of insertion			
Very easy at first attempt (no resistance)	70%	67%	NS
Easy at first attempt (little resistance)	27%	28%	NS
Difficult but successful at second attempt	3%	5%	NS
Not successful	—	—	
Insertion time within 20 s	97%	95%	NS
Mean cuff pressure, mmHg			
At start of surgery	45.0	45.0	NS
At end of surgery	100.3 ± 23.6	46.8 ± 3.6	<0.001
Blood on LM at time of removal, No.	4	0	NS

* Mann–Whitney U test.

LM = laryngeal mask; NS = not significant.

laryngeal mask insertion was only successful at the second attempt. The insertion of the Soft Seal LM became easier with time and experience. The laryngeal mask could be passed in the hypopharynx in all patients. In no case in either group did insertion of the laryngeal mask provoke laryngeal spasm or retching. No significant differences were seen in the hemodynamic and respiratory data in patients of both groups, and there were no events of desaturation during the trial. None of the patients needed a muscle relaxant at the time of insertion of the laryngeal mask. However, in 8% of the patients in the *LMA-Classic*TM group and 9% of the patients in the Soft Seal LM group, muscle relaxants were used because of surgical indications, but only well after the insertion and the clinical and fiberoptic evaluation of the laryngeal mask. Ventilation was well tolerated, and its use did not show any adverse effect, nor did it affect the results.

The mean laryngeal mask cuff pressure increased from 45 mmHg to 100.3 ± 23.6 mmHg in the *LMA-Classic*TM group and from 45 mmHg to 46.8 ± 3.6 mmHg in the Soft Seal LM group ($P < 0.001$) at the end of surgery (table 2). The presence of macroscopic blood on removal of the mask (4%) was only seen in the *LMA-Classic*TM group (table 2).

Sore throat at 2 h in the postoperative period was seen more frequently ($P < 0.05$) in the *LMA-Classic*TM group (20.5% vs. 10.2%; table 3). Mild sore throat, including dryness of the mouth, not requiring any treatment, was mentioned in 11 patients in the *LMA-Classic*TM group versus 10 in the Soft Seal group. In the *LMA-Classic*TM group, six patients had moderate pain, and three patients had severe pain of the throat. No statistically significant difference between the two groups at 24 h was observed (table 3).

At the time we checked the fiberoptic anatomic position of the laryngeal mask, we did not see any suspected or proved episodes of aspiration, regurgitation, or vom-

iting, although frequently, material was emerging from the trachea lumen into the hypopharynx, and saliva could be seen collecting in the hypopharynx. Although in 6% of the *LMA-Classic*TM and 4% of the Soft Seal LM cases the vocal cords could not be made visible by fiberoptic examination, satisfactory anesthesia was never a problem. The outcome of the fiberoptic examination did not reach statistical difference between the two groups (table 4).

Table 3. Comparison of Postoperative Sore Throat Incidence between Soft Seal LM Group and *LMA-Classic*TM Group at 2 h and at 24 h

	At 2 h	At 24 h
	<i>LMA-Classic</i> TM / Soft Seal LM	<i>LMA-Classic</i> TM / Soft Seal LM
Postoperative sore throat incidence		
None	79.5/89.8	80.3/86.3
Mild	11.4/10.2	9.2/14.7
Moderate	5.7/0	6.6/0
Severe	3.4/0	3.9/0
P value (Kruskal-Wallis test)	0.041	0.302 (NS)

LM = laryngeal mask; NS = not significant.

Table 4. Outcome of Fiberoptic Examination of Position of Two Laryngeal Masks

Epiglottis Position*	<i>LMA-Classic</i> TM , No.	Soft Seal LM, No.
Grade 4	51	43
Grade 3	31	47
Grade 2	12	6
Grade 1	6	4

* Not significant, Mann–Whitney U test ($P = 0.712$).

Discussion

This is the first report on the use of a new disposable laryngeal mask, the Soft Seal LM, in which we conducted a clinical comparison of the reusable *LMA-Classic™* and the new disposable Soft Seal LM size 4 and found that both laryngeal masks provided an adequate airway and similar clinical performance in spontaneously breathing patients. The Soft Seal LM was less traumatic, causing less sore throat in the early postoperative period.

Insertion Technique

It is a common practice to inflate the laryngeal mask cuff to the maximal recommended volume,³ while intracuff pressures are rarely measured and maintained in clinical practice. This often results in high intracuff pressures, up to 250 mmHg,¹⁷ possibly leading to increased mucosal pressure,^{2,27} pharyngolaryngeal trauma,^{13-14,27} and a suboptimal seal.³ In the past, we used this high recommended cuff volume practice until we found out that the majority of our patients had cuff pressures greater than 120 cm H₂O (90 mmHg) immediately after insertion of the laryngeal mask. Many authors now recommend inserting the laryngeal mask with the cuff partially inflated.^{3,11-18}

During anesthesia, a significant increase in cuff pressure is seen because of the presence of nitrous oxide, carbon dioxide, or other gases and because of the warming up of these gases. Avoiding high intracuff pressures and volumes during nitrous oxide anesthesia results in a better outcome for the patient (more optimal seal and less pharyngolaryngeal trauma).^{3,14-17} Some investigators show that high laryngeal mask pressures do not increase pharyngeal mucosal injury in dogs,²⁸ while others suggest reducing the cuff volume to a “just seal” situation.²⁹

We, too, believe that insertion of the laryngeal mask airway with the cuff partially inflated is equally successful to insert the laryngeal mask and results in a lower incidence of sore throat and pharyngeal mucosal bleeding. This might be the result of the presentation of a softer leading edge to the posterior pharyngeal wall.

Sore Throat

The incidence of sore throat using the *LMA-Classic™* in our study was 20%, which is identical to the findings of Brimacombe *et al.*¹⁵ when the cuff is partially inflated, compared to 42% if the cuff was fully inflated after insertion. Our incidence of sore throat with the Soft Seal LM is even lower (*i.e.*, 10%), which is similar to the incidence of sore throat after the use of a facemask (*i.e.*, 8%) in the studies of Brimacombe *et al.*¹⁵ and Dingley *et al.*³⁰

Using the standard approach technique, with the insertion of a noninflated *LMA-Classic™*, the reported incidence of sore throats ranges between 21.4% and 30%

according to Wakeling *et al.*,¹³ 28.5% in the study of Dingley *et al.*,³⁰ and up to 42% as measured by Brimacombe *et al.*¹⁵ The sore throat incidence is less when the cuff is partially inflated compared to noninflated cuffs, *i.e.*, 4.1% versus 21.4% as demonstrated by Wakeling *et al.*¹³

Materials

The Soft Seal LM is translucent, allowing easier visualization of any secretions inside it. On the disposable laryngeal mask, the size of the product and maximum cuff inflation volume are printed on the pilot balloon, allowing the clinician to recognize its size once *in situ* (fig. 1). Although the IDs of the *LMA-Classic™* and the Soft Seal LM are identical (11.0 mm), *in vitro* a 7.0-mm cuffed endotracheal tube can be inserted into the disposable laryngeal mask, while only a 6.0-mm endotracheal tube can be inserted into the shaft of the *LMA-Classic™*.

Fiberoptic Examination of the Position of the Laryngeal Mask

Patients with a “high” or “anterior” larynx did not always show a complete view of the larynx inlet by fiberoptic examination through the laryngeal mask in our study. However, the number of patients whose vocal cords were not visible was not significantly different between the two groups, confirming that insertion of both laryngeal masks results at least in the same position. All laryngeal masks used in this study resulted in adequate ventilation. This confirms that the absence of epiglottic bars have no deleterious effects on the performance of the laryngeal mask.³¹ Blockage of the airway tube by the epiglottis may be avoided by the deeper bowl, as is the case with the disposable laryngeal mask.

Limitations of the Study

We only compared size 4 laryngeal masks because this was the only size of disposable laryngeal mask available at the time of our study. For obvious financial reasons, we compared new disposable laryngeal masks with reusable *LMA-Classic™*. The *LMA-Classic™* may become more permeable to nitrous oxide the more it is used. The anatomic position of the LMA by fiberoptic evaluation was restricted to the view obtained from the tube of the laryngeal mask, limiting the results. We did not evaluate whether the use of a different lubricant on the LMA before insertion resulted in more or less pharyngolaryngeal trauma.

In conclusion, disposable laryngeal masks are an acceptable device to replace the reusable *LMA-Classic™*, resulting in a good laryngeal seal and similar clinical performance. The absence of epiglottic bars seems not to have deleterious effects on the performance of the laryngeal mask. Our study also shows that measuring cuff pressures of laryngeal masks may be advisable when

reusable *LMA-Classic™* masks are used, but this is unnecessary with the disposable Soft Seal LM.

The authors thank Marlies Schijven, M.D., Ph.D., Hsc. (Statistician, Department of Surgery, Catharina Hospital, Eindhoven, The Netherlands), for statistical analysis; Berry Bijsterveld and Jos Verbeek (Technicians, Catharina Hospital) for technical assistance; Guy Van Dael and Willem Binnendijk (Registered Medical Photographers, Audiovisual Department, Catharina Hospital) for audiovisual assistance; and the operating certified registered nurse anesthetists (Catharina Hospital) for their general assistance in this study.

References

1. Verghese C, Berlet J, Kapila A, Pollard R: Clinical assessment of the single use laryngeal mask airway: The LMA-Unique. *Br J Anaesth* 1998; 80:677-9
2. Keller C, Brimacombe J: Mucosal pressure, mechanism of seal, airway sealing pressure, and anatomic position for the disposable versus reusable laryngeal mask airways. *Anesth Analg* 1999; 88:1418-20
3. Brimacombe J, Keller C, Morris R, Mecklem D: A comparison of the disposable versus the reusable laryngeal mask airway in paralyzed adult patients. *Anesth Analg* 1998; 87:921-4
4. Maltby JR, Bériault MT, Watson NC, Liepert DJ, Fick GH: LMA-Classic™ and LMA-ProSeal™ are effective alternatives to endotracheal intubation for gynecologic laparoscopy. *Can J Anesth* 2003; 50:71-7
5. Miller DM, Youkhana I, Karunaratne WU, Pearce A: Presence of protein deposits on 'cleaned' re-usable anaesthetic equipment. *Anaesthesia* 2001; 56:1069-72
6. Parker MRJ, Day CJE: Visible and occult blood contamination of laryngeal mask airways and tracheal tubes used in adult anaesthesia. *Anaesthesia* 2000; 55:388-90
7. Tordoff SG, Scott S: Blood contamination of laryngeal mask airways and laryngoscopes: What to tell our patients? (letter) *Anaesthesia* 2002; 57:505-6
8. Smith G: Variant CJD: What you need to know at present. *The Royal College of Anaesthetists Bulletin* May 7, 2001:302-4
9. Chu LF, Trudell JR, Brock-Utne JG: Autoclaved reusable laryngeal mask airways contain significant protein contamination (abstract). *ANESTHESIOLOGY* 2002; 96:A570
10. Blunt MC, Burchett KR: Variant Creutzfeldt-Jacob disease and disposable anaesthetic equipment: Balancing the risks. Editorial. *Br J Anaesth* 2003; 90:1-3
11. Matta BF, Marsh DS, Nevin M: Laryngeal mask airway: A more successful method of insertion. *J Clin Anesth* 1995; 7:132-5
12. Dingley J, Asai T: Insertion methods of the laryngeal mask airway: A survey of current practice in Wales. *Anaesthesia* 1996; 51:596-9
13. Wakeling HG, Butler PJ, Baxter PJC: The laryngeal mask airway: A comparison between two insertion techniques. *Anesth Analg* 1997; 85:687-90
14. Brimacombe J, Holyoake L, Keller C, Barry J, Mecklem D, Blinco A, Weidmann K: Emergence characteristics and postoperative laryngopharyngeal morbidity with the laryngeal mask airway: A comparison of high versus low initial cuff volume. *Anaesthesia* 2000; 55:338-43
15. Brimacombe J, Holyoake L, Keller C, Brimacombe N, Scully M, Barry J, Talbutt P, Sartain J, McMahon P: Pharyngolaryngeal, neck, and jaw discomfort after anesthesia with the face mask and laryngeal mask airway at high and low cuff volumes in males and females. *ANESTHESIOLOGY* 2000; 93:26-31
16. McHardy FE, Chung F: Postoperative sore throat: Cause, prevention and treatment. *Anaesthesia* 1999; 54:444-53
17. Keller C, Pühringer F, Brimacombe JR: Influence of cuff volume on oropharyngeal leak pressure and fiberoptic position with the laryngeal mask airway. *Br J Anaesth* 1998; 81:186-7
18. O'Kelly SW, Heath KJ, Lawes EG: A study of laryngeal mask inflation. *Anaesthesia* 1993; 48:1075-8
19. Drage MP, Vaughan RS, Asai T: Jaw thrusting as a clinical test to assess the adequate depth of anaesthesia for insertion of the laryngeal mask. *Anaesthesia* 1996; 51:1167-70
20. Brain AJJ: Pressure in laryngeal mask airway cuffs (letter). *Anaesthesia* 1996; 51:603
21. Brimacombe J, Berry A, Brain AJJ: Optimal intracuff pressures with the laryngeal mask. *Br J Anaesth* 1996; 77:295-6
22. Keller C, Sparr HJ, Brimacombe JR: Laryngeal mask lubrication. *Anaesthesia* 1997; 52:592-7
23. Keller C, Brimacombe JR, Keller K, Morris R: Comparison of four methods for assessing airway sealing pressure with the laryngeal mask airway in adult patients. *Br J Anaesth* 1999; 82:286-7
24. Evans NR, Gardner SV, James MFM: ProSeal laryngeal mask protects against aspiration of fluid in the pharynx. *Br J Anaesth* 2002; 88:584-7
25. Joshi S, Sciacca RR, Solanki DR, Young WL, Mathru MM: A prospective evaluation of clinical tests for placement of laryngeal mask airways. *ANESTHESIOLOGY* 1998; 89:1141-6
26. Brimacombe J, Berry A: A proposed fiber-optic scoring system to standardize mask airway position (letter). *Anesth Analg* 1993; 76:457
27. Marjot R: Pressure exerted by the laryngeal mask airway cuff upon the pharyngeal mucosa. *Br J Anaesth* 1993; 70:25-9
28. Abud TM, Braz JR, Martins RH, Gregorio EA, Saldanha JC: High laryngeal mask airway pressures resulting from nitrous oxide do not increase pharyngeal mucosal injury in dogs. *Can J Anesth* 2001; 48:800-6
29. Rieger A, Brunne B: Is the laryngeal mask a minimally invasive instrument for securing the airway? *Anaesthesist* 1999; 48:399-402
30. Dingley J, Whitehead MJ, Wareham K: A comparative study of the incidence of sore throat with the laryngeal mask airway. *Anaesthesia* 1994; 49:251-4
31. Al-Shaikh B, Pilcher D: Is there a need for the epiglottic bars in the laryngeal mask airway? (letter) *Can J Anesth* 2003; 50:203-4