

# Impact of Bone Quality and Implant Type on the Primary Stability: An Experimental Study Using Bovine Bone

Sukumaran Anil, BDS, MDS, PhD<sup>1\*</sup>

Abdullah Alfarraj Aldosari, BDS, DMSc<sup>2</sup>

The purpose of this in vitro study was to compare the primary stability and removal torque of bone level and tissue level implants in different bone qualities. Twenty tissue level and bone level implants ( $3.3 \times 10$  mm and  $4.1 \times 10$  mm) were used for assessing the stability in type II and type IV bone. Forty bovine rib blocks were used in this study. The primary stability of the implant was measured by the resonance frequency using an Osstel device. The removal torque values (RTV) of the implants was assessed using a digital torque gauge instrument. The implant stability quotient (ISQ) values and the RTV showed a marginally higher stability with bone level implants as compared to tissue level implants. However, these differences were not statistically significant in both type of bone used ( $P > 0.05$ ). On the other hand, compared to type IV, type II bone showed significant differences in the ISQ ( $P < 0.01$ ) and RTV ( $P < 0.001$ ) of bone level and tissue level implants. The study concluded that bone quality is an important factor in establishing primary stability than the implant dimension. Bone level and tissue level implants of same dimensions can be selected based on the esthetic demands since they showed similar mechanical properties.

**Key Words:** implants, removal torque, primary stability, osseointegration, resonance frequency analysis

## INTRODUCTION

Successful osseointegration has an important influence on the long-term success of dental implant restorations. While primary implant stability and osseointegration can be predictably achieved in dense bone, it is often challenging to achieve the same in areas with poor bone quality.<sup>1</sup> Primary stability lowers the level of implant micromotion, which in turn allows uninhibited healing and osseointegration.<sup>2</sup> Friberg et al<sup>3</sup> reported an implant failure rate of 32% for those implants that showed inadequate initial stability.

Studies have demonstrated that initial implant stability is influenced by factors such as the length and diameter of the implant, the implant design, the micromorphology of the implant surface, the insertion technique, and the congruity between the implant and the surrounding bone.<sup>4-7</sup> Further important determinants are the quality and quantity of the bone. Low density bone implant sites have been pointed out as the greatest potential risk factor for implant loss when working with standard bone drilling protocols.<sup>8,9</sup> Clinical studies with consecutively placed implants that were immediately loaded showed a higher failure rate in low density bone, reinforcing that primary stability is a major determinant in the success of immediately loaded implants.<sup>10,11</sup>

The success of implant depends on the bone quality and the healing at the implant-bone interface. The structural and

material properties of bone such as mineral density and mineral maturity are important contributors to bone strength.<sup>12,13</sup> Even though majority of literature defines the bone quality in terms of bone density, other biological factors such as bone metabolism, cell turnover, mineralization, maturation, intercellular matrix, and vascularity also influence the osseointegration.<sup>11,12</sup> The stiffness of the bone around the implant increases during the process of osseointegration, and the interlocks between bones and implant surface prevents micromotion and formation of fibrous scar tissue when the implant is loaded properly.<sup>14,15</sup> Basically, the stability of implants is largely associated with osseointegration and peri-implant bone remodeling during healing process.

Bone level implants were introduced by the International Team for Implantology to minimize crestal bone loss and to improve the esthetic predictability of implant-based restorations. The biomechanical properties of these implants are not thoroughly explored. Also, the claim that these implants have lesser crestal bone loss compared to tissue level implants is controversial. The reason for this controversy is that implant abutment junction (microgap) is closer to the bone, which may result in more bone loss. However, in terms of esthetic point of view, bone level implants are superior to tissue level implants.<sup>16</sup>


Numerous methods are used to assess the primary stability of the dental implant.<sup>17</sup> Among these resonance frequency analysis has been found to be the most successful method to assess primary stability because of its easiness, accuracy, and noninvasiveness.<sup>1,18</sup> The implant-bone interface is measured by resonance frequency (RF), which is the reaction to oscillations exerted to the implant. The result is expressed as the implant stability quotient (ISQ).<sup>19</sup> However, a mechanical test—such as insertion torque and values of push-out test—showed positive

<sup>1</sup> Department of Periodontics and Community Dentistry, College of Dentistry, King Saud University, Riyadh, Saudi Arabia.

<sup>2</sup> Department of Prosthetic Science, Dental Implant and Osseointegration Research Chair, College of Dentistry, King Saud University, Riyadh, Saudi Arabia.

\* Corresponding author, e-mail: drsanil@gmail.com

DOI: 10.1563/AAID-JOI-D-11-00156

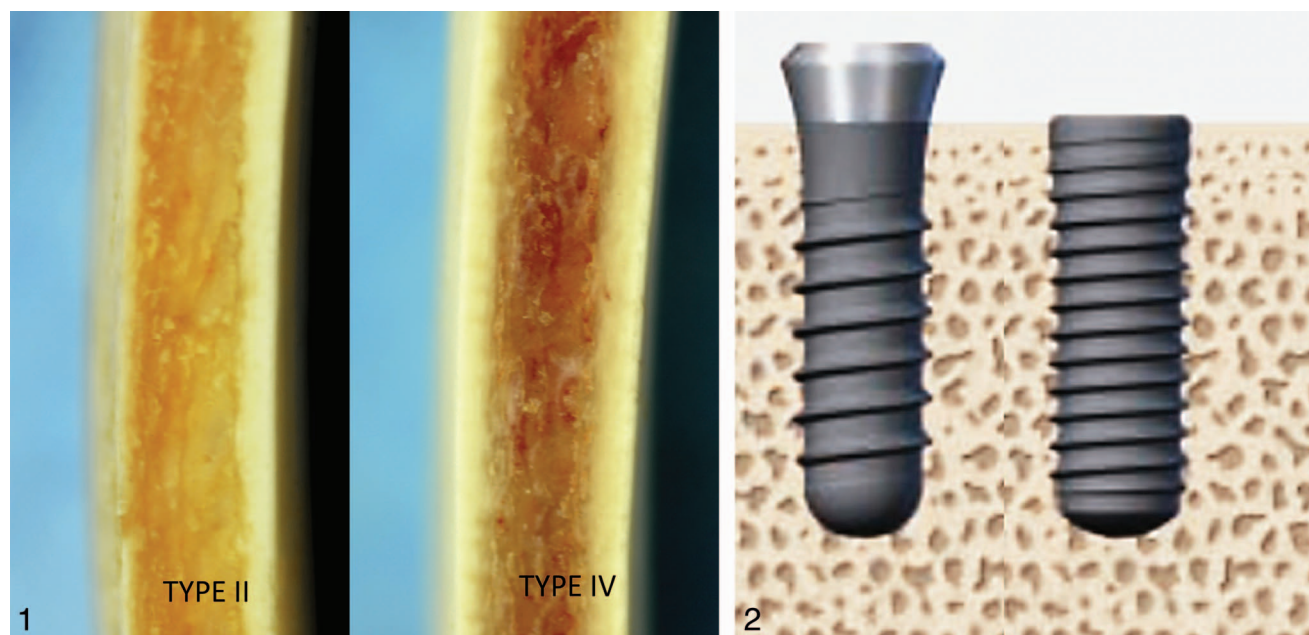

**FIGURES 1 AND 2.** **FIGURE 1.** The bovine rib showing type II and type IV bone. **FIGURE 2.** Illustration showing the positioning of tissue level and bone level implants.

correlation to the primary stability.<sup>20,21</sup> Hence, noninvasive measurement methods have been introduced for the diagnosis and prediction of immediate and the long-term implant stability. Studies have shown that the measurement of removal torque strength was a useful indirect biomechanical method to evaluate the bone and implant interface.<sup>22,23</sup> The purpose of this in vitro study is to compare the primary stability and removal torque measurements of bone level and tissue level implants in different bone qualities.

#### MATERIALS AND METHODS

Fresh bovine ribs procured from the butcher shop were used for the study. They were cut into 6 cm-long pieces, and a total of 40 bovine rib blocks were prepared. The cortical bone was removed in 20 blocks until it was about 1 mm thick to make it mimic type II bone.<sup>24</sup> The other 20 blocks had all cortical bone removed and the trabecular bone exposed to make it similar to type IV bone (Figure 1). Twenty tissue level (standard plus) and 20 bone level implants with 2 different dimensions ( $3.3 \times 10$  and  $4.1 \times 10$ ) were installed in each rib blocks (Figure 2).

#### Resonance frequency (RF)

After installation, the ISQ was measured by using resonance frequency analyzer (Osstell, Osstell AB, Göteborg, Sweden). The osteotomy sites were prepared according to the manufacturer's guidelines. After implant insertion, the magnetic wireless RF analyzer was used for direct measurement of the endosseous implant stability. The RF analysis technique analyzes the RF range (110–10000 Hz) of a SmartPeg, which can be attached to the implant. The probe of wireless RF analyzer Osstell Mentor was held perpendicular to the implant as indicated by the manufacturer (Figure 3).

#### Removal torque values (RTV)

The RTV of each implant was measured using a MGT 50 digital torque gauge instrument (MARK-10 Corp., New York). A controlled, gradually increasing rotational force (displacement 0.5 mm min<sup>-1</sup>) was applied to the implant until implant loosening (Figure 4). The peak force measured at implant loosening was scored as the torque-out value.<sup>25</sup>



#### Statistical analysis

The statistical analysis was performed with GraphPad Instat 3.05 software (GraphPad Software Inc, San Diego, Calif) using analysis of variance (ANOVA). The Tukey-Kramer multiple comparisons test was used to compare the ISQ values and RTV of the two types of implants with two different dimensions. *P*-values < 0.05 were assumed to be statistically significant.

#### RESULTS

The mean values and standard deviations of resonance frequency measurements are shown in Figure 5. Bone level implants showed ISQ values of  $67.35 \pm 5.21$  and  $71.65 \pm 5.85$ , respectively, for the 3.3 and 4.1 diameter implants. These values were higher than tissue level implants of the same dimensions. Similar results were also found in type IV bone (Figure 5). Compared to type IV bone, the primary stability of type II bone showed significantly higher values (*P* < 0.01) for the 3.3 and 4.1 diameter implants.

The removal torque values are depicted in Figure 6. The removal torque measurements showed no significant differences between bone level and tissue level implants with the 2 different dimensions of the implants used (Figure 6). However, significantly lower removal torque values were observed in type IV bone as compared to the type II bone (*P* < 0.001).

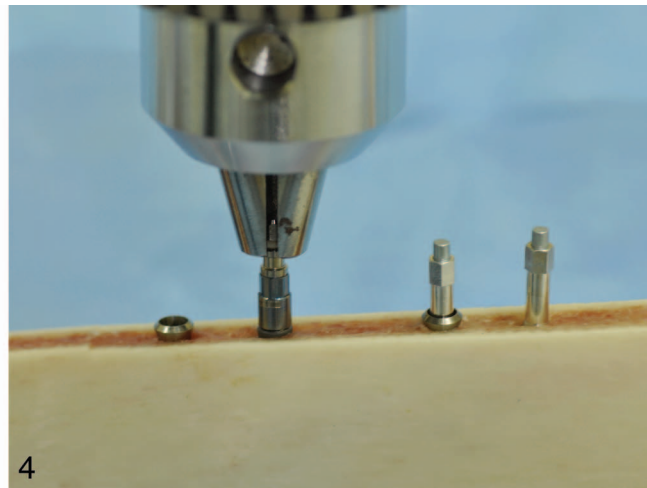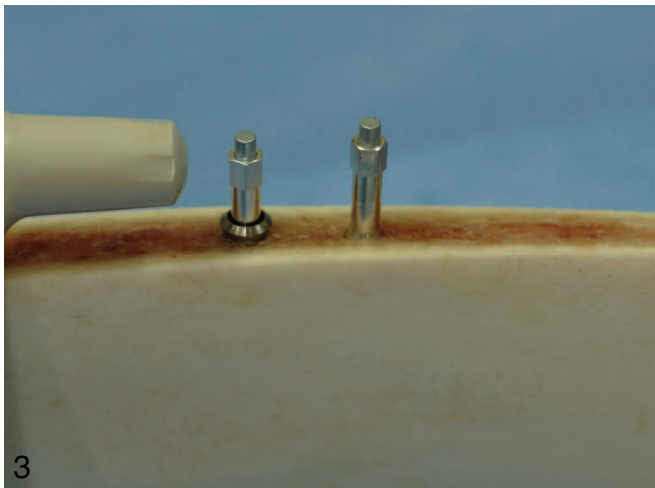

**FIGURES 3 AND 4.** **FIGURE 3.** The implant in position with the SmartPeg and the tip of the Osstel Mentor resonance frequency analyser. **FIGURE 4.** The positioning of the digital torque gauge.

**DISCUSSION**



Implant stability is a prerequisite for the long-term clinical success of osseointegrated implants.<sup>26,27</sup> The stability of implants can be successfully assessed by the Osstel device, which quantifies the RF. Resonance frequency is a noninvasive, objective method to evaluate implant stability, and it has been validated through in vitro and in vivo studies.<sup>19,28</sup> The technique is based on the measurement of the RF of a small piezoelectric transducer attached to an implant or abutment.<sup>19,29</sup>

It is well known that primary stability of implants depends on surgical techniques used, bone density, and implant design.<sup>30-32</sup> Maintenance of low implant micro-movement, especially in the early healing phase, is important to promote direct bone in growth to implant surface.<sup>33</sup> Earlier studies have shown a linear relationship between the exposed implant height and the corresponding ISQ values.<sup>21,34</sup> Sim and Lang<sup>35</sup>

reported a correlation between the ISQ values and the bone structure and implant length. However, O’Sullivan et al<sup>36</sup> failed to report any correlation between the implant primary stability and the shape of the implant. In the present study, a comparison was done between bone level implants and tissue level implants with similar dimensions. Bone level implants showed slightly higher but insignificant ISQ and removal torque values as compared to the tissue level implants.

However, when the primary stability of implants were compared in different bone qualities, statistically higher ISQ values were observed for implants inserted in type II bone with 1 mm cortical bone. This observation is in agreement with observation of Akca et al,<sup>37</sup> who reported that bone quality had more influence than implant shape. Elias et al<sup>15</sup> concluded that implant design, surgical technique, and substrate type are the major components influencing the primary stability.

Bovine rib was used in this study and is classified as type II bone in other studies because it contains thick compact bone

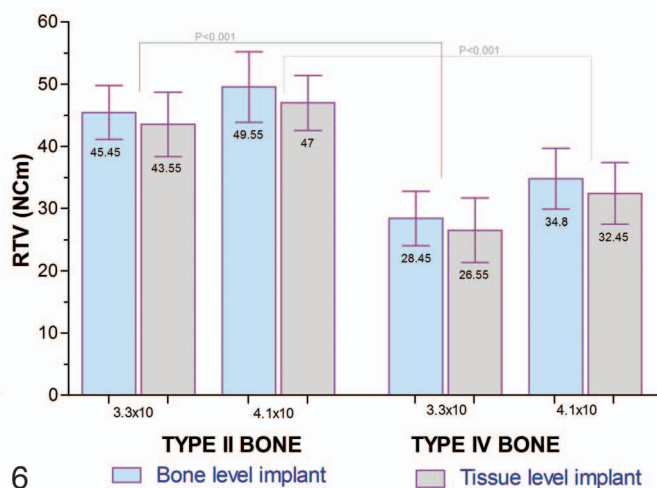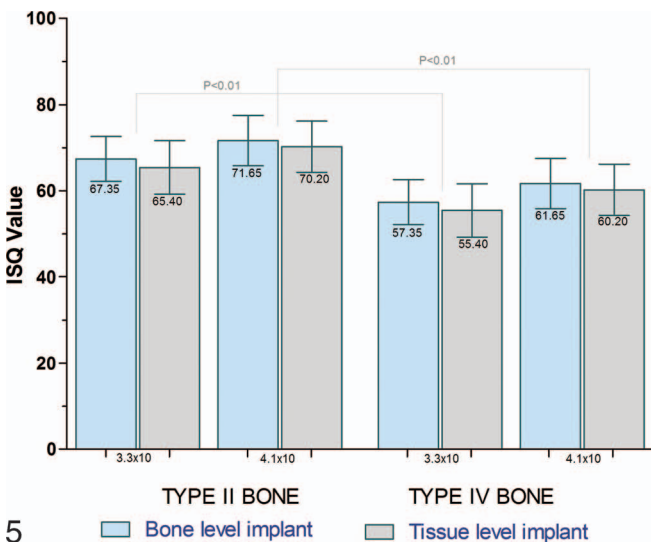

**FIGURES 5 AND 6.** **FIGURE 5.** The RF values (ISQ) of bone level and tissue level implants in type II and type IV bone. **FIGURE 6.** The removal torque values (RTV) of bone level and tissue level implants in type II and type IV bone.



and dense trabecular bone.<sup>38</sup> To mimic the type IV bone, the entire cortical bone is removed. The lower ISQ values and removal torque observed in this experiment indicates that the bone quality is an important determinant in the early implant stability. There were significant correlations between bone density and removal torque values, which is in agreement with earlier studies.<sup>39,40</sup>

To evaluate the initial bone quality and degree of osseointegration, various methods have been proposed,<sup>41</sup> including histology and histomorphometry,<sup>42–45</sup> removal torque analysis,<sup>46–48</sup> pull- and push-through tests,<sup>49</sup> and X-ray examination.<sup>30</sup> RFA has been used to study the factors—including surgical technique, loading protocol, and implant design—that govern implant stability. Implant stability can also vary with a change in osseous remodeling and percentage of implant bone interface contact.<sup>50</sup> The major drawback of the RFA analysis is that it can reflect only the mechanical property of the bone-implant interfacial layer by assessing the changes of stiffness during the osseointegration process.<sup>29,41,51</sup> Even though it is an excellent nondestructive method, its clinical application is limited to establish the implant stability and the prognostic criteria for long-term implant success.<sup>52,53</sup>

### CONCLUSION

Within the limitations of the study, it can be assumed that bone quality is an important factor in establishing primary stability than the implant dimension from the biomechanical point. The main limitation of the present study is that the mechanical characteristics of the primary stability of an implant were considered in an in vitro setup using bovine bone. Further in vivo studies are required to understand the actual clinical situation in which many biological factors influence the primary stability of implants. Moreover, secondary stability tests, finite element studies, and histomorphometric studies are necessary to substantiate the present observations.<sup>54</sup> The priority for selecting either a bone level or a tissue level implant of same dimension should be based on esthetic demands, since they show similar mechanical properties.

### ABBREVIATIONS

ISQ: implant stability quotient  
RF: resonance frequency  
RFA: resonance frequency analysis  
RTV: removal torque values

### ACKNOWLEDGMENT

The authors would like to extend their sincere appreciation to the Deanship of Scientific Research, King Saud University, for funding this research.

### REFERENCES

1. Yoon HG, Heo SJ, Koak JY, Kim SK, Lee SY. Effect of bone quality and implant surgical technique on implant stability quotient (ISQ) value. *J Adv Prosthodont*. 2011;3:10–15.

2. Traini T, Assenza B, Roman F, Thams U, Caputi S, Piattelli A. Bone microvascular pattern around loaded dental implants in a canine model. *Clin Oral Invest*. 2006;10:151–156.
3. Friberg B, Jemt T, Lekholm U. Early failures in 4,641 consecutively placed Branemark dental implants: a study from stage 1 surgery to the connection of completed prostheses. *Int J Oral Maxillofac Implants*. 1991;6:142–146.
4. O'Sullivan D, Sennerby L, Jagger D, Meredith N. A comparison of two methods of enhancing implant primary stability. *Clin Implant Dent Relat Res*. 2004;6:48–57.
5. Abrahamsson I, Linder E, Lang NP. Implant stability in relation to osseointegration: an experimental study. *Clin Oral Implants Res*. 2009;20:313–318.
6. Büchter A, Kleinheinz J, Joos U, Meyer U. Primary implant stability with different bone surgery techniques. An in vitro study of the mandible of the minipig. *Mund-, Kiefer-und Gesichtschirurgie: MKG*. 2003;7:351.
7. Cicciu M, Risitano G, Maiorana C, Franceschini G. Parametric analysis of the strength in the "Toronto" osseous-prosthesis system. *Minerva Stomatol*. 2009;58:9–23.
8. Jacobs R. Preoperative radiologic planning of implant surgery in compromised patients. *Periodontol 2000*. 2003;33:12–25.
9. Garg AK. Success of dental implants in the geriatric patient. *Dent Implantol Update*. 2002;13:25–31.
10. Glauser R, Ree A, Lundgren A, Gottlow J, Hämmerle CH, Schärer P. Immediate occlusal loading of Branemark implants applied in various jawbone regions: a prospective, 1-year clinical study. *Clin Implant Dent Relat Res*. 2001;3:204–213.
11. Molly L. Bone density and primary stability in implant therapy. *Clin Oral Implants Res*. 2006;17(suppl 2):124–135.
12. Paschalis EP, Tatakis DN, Robins S, et al. Lathyism-induced alterations in collagen cross-links influence the mechanical properties of bone material without affecting the mineral. *Bone*. 2011;49:1232–1241.
13. Fratzl P, Gupta H, Paschalis E, Roschger P. Structure and mechanical quality of the collagen-mineral nano-composite in bone. *J Mater Chem*. 2004;14:2115–2123.
14. Sennerby L, Meredith N. Implant stability measurements using resonance frequency analysis: biological and biomechanical aspects and clinical implications. *Periodontol 2000*. 2008;47:51–66.
15. Elias CN, Rocha FA, Nascimento AL, Coelho PG. Influence of implant shape, surface morphology, surgical technique, and bone quality on the primary stability of dental implants. *J Mech Behav Biomed Mater*. 2012;16:169–180.
16. Buser D, Schmid B, Belser UC, Cochran DL. The new bone level implants—clinical rationale for the development and current indications for daily practice. *International Dentistry SA*. 2010;12:58–64.
17. Lachmann S, Jager B, Axmann D, Gomez-Roman G, Groten M, Weber H. Resonance frequency analysis and damping capacity assessment. Part I: an in vitro study on measurement reliability and a method of comparison in the determination of primary dental implant stability. *Clin Oral Implants Res*. 2006;17:75–79.
18. Balleri P, Cozzolino A, Ghelli L, Momicchioli G, Varriale A. Stability measurements of osseointegrated implants using Osstell in partially edentulous jaws after 1 year of loading: a pilot study. *Clin Implant Dent Relat Res*. 2002;4:128–132.
19. Meredith N. A review of nondestructive test methods and their application to measure the stability and osseointegration of bone anchored endosseous implants. *Crit Rev Biomed Eng*. 1998;26:275–291.
20. Degidi M, Perrotti V, Strocchi R, Piattelli A, Iezzi G. Is insertion torque correlated to bone-implant contact percentage in the early healing period? A histological and histomorphometrical evaluation of 17 human-retrieved dental implants. *Clin Oral Implants Res*. 2009;20:778–781.
21. Turkyilmaz I, Sennerby L, McGlumphy EA, Tozum TF. Biomechanical aspects of primary implant stability: a human cadaver study. *Clin Implant Dent Relat Res*. 2009;11:113–119.
22. Carlsson L, Rostlund T, Albrektsson B, Albrektsson T. Removal torques for polished and rough titanium implants. *Int J Oral Maxillofac Implants*. 1988;3:21–24.
23. Motoyoshi M, Hirabayashi M, Uemura M, Shimizu N. Recommended placement torque when tightening an orthodontic mini-implant. *Clinical oral implants research*. 2006;17:109–114.
24. Lekholm U, Zarb G, Branemark P, Zarb G. *Tissue Integrated Prostheses Osseointegration in Clinical Dentistry*. Chicago: Quintessence; 1985.
25. Schouten C, Meijer GJ, van den Beucken JJ, et al. In vivo bone response and mechanical evaluation of electrosprayed CaP nanoparticle

coatings using the iliac crest of goats as an implantation model. *Acta Biomater.* 2010;6:2227–2236.

26. Seong WJ, Kim UK, Swift JQ, Hodges JS, Ko CC. Correlations between physical properties of jawbone and dental implant initial stability. *J Prosthet Dent.* 2009;101:306–318.

27. Dilek O, Tezulas E, Dincel M. Required minimum primary stability and torque values for immediate loading of mini dental implants: an experimental study in nonviable bovine femoral bone. *Oral Surg Oral Med Oral Pathol Oral Radiol Endod.* 2008;105:e20–e27.

28. Veltri M, Balleri P, Ferrari M. Influence of transducer orientation on Osstell stability measurements of osseointegrated implants. *Clin Implant Dent Relat Res.* 2007;9:60–64.

29. Meredith N, Alleyne D, Cawley P. Quantitative determination of the stability of the implant-tissue interface using resonance frequency analysis. *Clin Oral Implants Res.* 1996;7:261–267.

30. Meredith N. Assessment of implant stability as a prognostic determinant. *Int J Prosthodont.* 1998;11:491–501.

31. Alghamdi H, Anand PS, Anil S. Undersized implant site preparation to enhance primary implant stability in poor bone density: a prospective clinical study. *J Oral Maxillofac Surg.* 2011;69:e506–e512.

32. Al-Marshood MM, Junker R, Al-Rasheed A, Al Farraj Aldosari A, Jansen JA, Anil S. Study of the osseointegration of dental implants placed with an adapted surgical technique. *Clin Oral Implants Res.* 2011;22:753–759.

33. Szmukler-Moncler S, Salama H, Reingewirtz Y, Dubruille JH. Timing of loading and effect of micromotion on bone-dental implant interface: review of experimental literature. *J Biomed Mater Res.* 1998;43:192–203.

34. Tozum TF, Turkyilmaz I, McGlumphy EA. Relationship between dental implant stability determined by resonance frequency analysis measurements and peri-implant vertical defects: an in vitro study. *J Oral Rehabil.* 2008;35:739–744.

35. Sim CP, Lang NP. Factors influencing resonance frequency analysis assessed by Osstell mentor during implant tissue integration: I. Instrument positioning, bone structure, implant length. *Clin Oral Implants Res.* 2010;21:598–604.

36. O'Sullivan D, Sennerby L, Meredith N. Measurements comparing the initial stability of five designs of dental implants: a human cadaver study. *Clin Implant Dent Relat Res.* 2000;2:85–92.

37. Akca K, Akkocaoglu M, Comert A, Tekdemir I, Cehreli MC. Bone strains around immediately loaded implants supporting mandibular overdentures in human cadavers. *Int J Oral Maxillofac Implants.* 2007;22:101–109.

38. Trisi P, Perfetti G, Baldoni E, Berardi D, Colagiovanni M, Scogna G. Implant micromotion is related to peak insertion torque and bone density. *Clin Oral Implants Res.* 2009;20:467–471.

39. Beer A, Gahleitner A, Holm A, Tschabitscher M, Homolka P. Correlation of insertion torques with bone mineral density from dental quantitative CT in the mandible. *Clin Oral Implants Res.* 2003;14:616–620.

40. Akca K, Chang TL, Tekdemir I, Fanuscu MI. Biomechanical aspects of

initial intraosseous stability and implant design: a quantitative micro-morphometric analysis. *Clin Oral Implants Res.* 2006;17:465–472.

41. Huang HM, Chiu CL, Yeh CY, Lin CT, Lin LH, Lee SY. Early detection of implant healing process using resonance frequency analysis. *Clin Oral Implants Res.* 2003;14:437–443.

42. Albrektsson T, Jacobsson M. Bone-metal interface in osseointegration. *J Prosthet Dent.* 1987;57:597–607.

43. Sennerby L, Thomsen P, Ericson LE. A morphometric and biomechanic comparison of titanium implants inserted in rabbit cortical and cancellous bone. *Int J Oral Maxillofac Implants.* 1992;7:62–71.

44. Sennerby L, Thomsen P, Ericson LE. Ultrastructure of the bone-titanium interface in rabbits. *J Mater Sci Mater Med.* 1992;3:262–271.

45. Ericsson I, Johansson CB, Bystedt H, Norton MR. A histomorphometric evaluation of bone-to-implant contact on machine-prepared and roughened titanium dental implants. A pilot study in the dog. *Clin Oral Implants Res.* 1994;5:202–206.

46. Carlsson L, Rostlund T, Albrektsson B, Albrektsson T. Removal torques for polished and rough titanium implants. *Int J Oral Maxillofac Implants.* 1988;3:21–24.

47. Johansson CB, Sennerby L, Albrektsson T. A removal torque and histomorphometric study of bone tissue reactions to commercially pure titanium and Vitallium implants. *Int J Oral Maxillofac Implants.* 1991;6:437–441.

48. Wennerberg A, Albrektsson T, Andersson B, Krol JJ. A histomorphometric and removal torque study of screw-shaped titanium implants with three different surface topographies. *Clin Oral Implants Res.* 1995;6:24–30.

49. Dhert WJ, Verheyen CC, Braak LH, et al. A finite element analysis of the push-out test: influence of test conditions. *J Biomed Mater Res.* 1992;26:119–130.

50. Deng B, Tan KB, Liu GR, Lu Y. Influence of osseointegration degree and pattern on resonance frequency in the assessment of dental implant stability using finite element analysis. *Int J Oral Maxillofac Implants.* 2008;23:1082–1088.

51. Natali AN, Pavan PG, Schileo E, Williams KR. A numerical approach to resonance frequency analysis for the investigation of oral implant osseointegration. *J Oral Rehabil.* 2006;33:674–681.

52. Becker W, Sennerby L, Bedrossian E, Becker BE, Lucchini JP. Implant stability measurements for implants placed at the time of extraction: a cohort, prospective clinical trial. *J Periodontol.* 2005;76:391–397.

53. Ersanli S, Karabuda C, Beck F, Leblebicioglu B. Resonance frequency analysis of one-stage dental implant stability during the osseointegration period. *J Periodontol.* 2005;76:1066–1071.

54. Lee JH, Frias V, Lee KW, Wright RF. Effect of implant size and shape on implant success rates: a literature review. *J Prosthet Dent.* 2005;94:377–381.