



# Reduction in Hypoglycemia With the Predictive Low-Glucose Management System: A Long-term Randomized Controlled Trial in Adolescents With Type 1 Diabetes

*Diabetes Care* 2018;41:303–310 | <https://doi.org/10.2337/dc17-1604>

Mary B. Abraham,<sup>1–3</sup>  
Jennifer A. Nicholas,<sup>1,2</sup> Grant J. Smith,<sup>2</sup>  
Janice M. Fairchild,<sup>4</sup> Bruce R. King,<sup>5</sup>  
Geoffrey R. Ambler,<sup>6</sup> Fergus J. Cameron,<sup>7</sup>  
Elizabeth A. Davis,<sup>1–3</sup> and  
Timothy W. Jones,<sup>1–3</sup> on behalf of the  
PLGM Study Group\*

## OBJECTIVE

Short-term studies with automated systems that suspend basal insulin when hypoglycemia is predicted have shown a reduction in hypoglycemia; however, efficacy and safety have not been established in long-term trials.

## RESEARCH DESIGN AND METHODS

We conducted a 6-month, multicenter, randomized controlled trial in children and adolescents with type 1 diabetes using the Medtronic MiniMed 640G pump with Suspend before low (predictive low-glucose management [PLGM]) compared with sensor-augmented pump therapy (SAPT) alone. The primary outcome was percentage time in hypoglycemia with sensor glucose (SG) <3.5 mmol/L (63 mg/dL).

## RESULTS

In an intent-to-treat analysis of 154 subjects, 74 subjects were randomized to SAPT and 80 subjects to PLGM. At baseline, the time with SG <3.5 mmol/L was 3.0% and 2.8% in the SAPT and PLGM groups, respectively. During the study, PLGM was associated with a reduction in hypoglycemia compared with SAPT (% time SG <3.5 mmol/L: SAPT vs. PLGM, 2.6 vs. 1.5,  $P < 0.0001$ ). A similar effect was also noted in time with SG <3 mmol/L ( $P < 0.0001$ ). This reduction was seen both during day and night ( $P < 0.0001$ ). Hypoglycemic events (SG <3.5 mmol/L for >20 min) also declined with PLGM (SAPT vs. PLGM: events/patient-year 227 vs. 139,  $P < 0.001$ ). There was no difference in glycated hemoglobin (HbA<sub>1c</sub>) at 6 months (SAPT 7.6 ± 1.0% vs. PLGM 7.8 ± 0.8%,  $P = 0.35$ ). No change in quality of life measures was reported by participants/parents in either group. There were no PLGM-related serious adverse events.

## CONCLUSIONS

In children and adolescents with type 1 diabetes, PLGM reduced hypoglycemia without deterioration in glycemic control.

<sup>1</sup>Children's Diabetes Centre, Telethon Kids Institute, The University of Western Australia, Perth, Australia

<sup>2</sup>Department of Endocrinology and Diabetes, Princess Margaret Hospital for Children, Perth, Australia

<sup>3</sup>Division of Paediatrics, Medical School, The University of Western Australia, Perth, Australia

<sup>4</sup>Department of Endocrinology and Diabetes, Women's and Children's Hospital, Adelaide, Australia

<sup>5</sup>Department of Endocrinology and Diabetes, John Hunter Children's Hospital, Newcastle, Australia

<sup>6</sup>Institute of Endocrinology and Diabetes, The Children's Hospital at Westmead and Clinical School, The University of Sydney, Sydney, Australia

<sup>7</sup>Department of Endocrinology and Diabetes, The Royal Children's Hospital, Melbourne, Australia

Corresponding author: Timothy W. Jones, [tim.jones@health.wa.gov.au](mailto:tim.jones@health.wa.gov.au).

Received 2 August 2017 and accepted 31 October 2017.

Clinical trial reg. no. ACTRN12614000510640, [www.anzctr.org.au](http://www.anzctr.org.au).

This article contains Supplementary Data online at <http://care.diabetesjournals.org/lookup/suppl/doi:10.2337/dc17-1604/-/DC1>.

\*A complete list of the members of the PLGM Study Group can be found in the Supplementary Data online.

© 2017 by the American Diabetes Association. Readers may use this article as long as the work is properly cited, the use is educational and not for profit, and the work is not altered. More information is available at <http://www.diabetesjournals.org/content/license>.

The integration of real-time continuous glucose monitoring (CGM) systems and pump therapy has been an important milestone in the management of type 1 diabetes (1), and the more recent incorporation of control algorithms has offered potential to further improve clinical outcomes. For example, the “Low glucose suspend” algorithm shuts off basal insulin delivery with sensor-detected hypoglycemia and has been shown to reduce the duration and severity of hypoglycemia (2,3). The next step has been the development of an algorithm that predicts impending hypoglycemia based on CGM and suspends basal insulin before the occurrence of hypoglycemia. The predictive low-glucose management (PLGM) system, the only commercially available sensor-integrated insulin delivery system, has been shown to reduce hypoglycemia in in-clinic conditions (4–6), in short-term outpatient observational studies (7–11), and recently in a 2-week randomized controlled trial (12). The important question as to whether the system is effective and safe in long-term use, and by inference in clinical practice, is however untested, especially as long-term CGM use has been challenging for many patients. Short-term studies have not provided information as to whether the system results in deterioration in glycemic control. Finally, it is not known whether behavioral changes develop in an individual using these systems over the long term and whether these in turn will impact on outcomes. A 6-month study attempts to address these questions.

The PLGM system is incorporated in the MiniMed 640G pump (Medtronic, Northridge, CA). The pump, when used in conjunction with the Medtronic Enlite Sensor and Guardian 2 Link transmitter, has the “Suspend before low” feature, which suspends insulin infusion when hypoglycemia is predicted. In order to test the effectiveness and safety of the system over the long term, we conducted a 6-month randomized controlled home trial in real-life conditions in older children and adolescents. This age-group is at significant risk of hypoglycemia (13) and in most surveys has higher glycated hemoglobin (HbA<sub>1c</sub>) and potentially has the most to gain from strategies that potentially could improve glycemic control.

## RESEARCH DESIGN AND METHODS

### Study Design and Participants

A detailed description of the study protocol has been published (14). This was a

multicenter, unblinded, parallel, randomized controlled phase 3 home trial conducted by five tertiary pediatric diabetes centers in Australia. Ethics approval was received at each site. Eligible patients were 8–20 years of age, had type 1 diabetes of at least 1 year duration, with HbA<sub>1c</sub> of <10% (<86 mmol/mol), and had used insulin pump therapy for >6 months. Patients were excluded if they had any medical condition predisposing to hypoglycemia, were on oral hypoglycemic agents, were pregnant, or were not able to comply and meet the protocol requirements. Participants were screened through the diabetes clinics for eligibility in the study. Written informed consent was obtained from participants aged ≥18 years and written parental consent and participant assent for those <18 years of age.

Participants were randomized to either the control group with sensor-augmented pump therapy (SAPT) alone (Suspend on low and Suspend before low not enabled) or to the intervention group with SAPT and Suspend before low enabled (PLGM). Participants were allocated to either SAPT or PLGM using minimization incorporating a random element. Each site had its own minimization schedule based on the following equally weighted factors: sex, age, HbA<sub>1c</sub>, and hypoglycemia awareness score. Participants were allocated to the minimization-preferred group at a probability of 0.7. The program Minimp (version 0.3) was used to allocate participants (15).

### PLGM System

The “Suspend before low” feature is a SmartGuard function on the MiniMed 640G pump. The low limit was set for the entire study duration at 3.4 mmol/L (61 mg/dL), and the pump would therefore suspend insulin infusion when sensor glucose (SG) was ≤7.3 mmol/L or 131 mg/dL (70 mg/dL above the low limit) and predicted to be ≤4.5 mmol/L or 81 mg/dL (20 mg/dL above the low limit) in 30 min. In the absence of patient interference, after pump suspension, the insulin infusion resumes after a maximum suspend period of 2 h or earlier if the autoresumption parameters are met. The low-limit alarm was by default active when PLGM was on. In the control group on SAPT, all participants were advised to keep the low-limit alarm on. In both groups, the alerts on high, before high, and before low were optional for the

participant. The basal resume alert (on autoresumption) was an optional alert in patients using PLGM; however, the system always alerted the patient if basal infusion resumed after the 2-h maximum suspend period.

### Study Visits

The first and second visits were for pump start and sensor training, respectively. A minimum of a 2-week run-in period was required to demonstrate confidence in using the system and to ensure eligibility for randomization. All participants were required to use CGM for >80% of the time and demonstrate hypoglycemia (at least one SG <3.5 mmol/L) or risk of hypoglycemia (one or more SG <4.4 mmol/L on at least three different days). At visit three, eligible participants were randomly assigned to standard SAPT or PLGM. The study visit schedule was identical in both groups, and the participants were followed up at 3 and 6 months after randomization (visits four and five). Pump data were uploaded to Medtronic CareLink Therapy Management Software for Diabetes. HbA<sub>1c</sub> levels were measured at randomization and at visits four and five. Validated questionnaires were administered to participants and/or their parents at the first visit and repeated at visits four and five. These included the hypoglycemia awareness questionnaire from Clarke et al. (16), EQ-5D-Y and pediatric-specific diabetes quality of life (PedsQL) questionnaires (17), hypoglycemia fear survey (18), and CGM satisfaction questionnaire (19). Apart from ketone testing as part of routine care during sick days, participants were instructed to test for ketones before breakfast and prebed in both groups and after pump resumption after 2 h of suspend in the intervention group during the awake hours.

### Study Outcomes

The primary objective of the study was the comparison of the average percentage of time spent in hypoglycemia (SG <3.5 mmol/L) with PLGM versus SAPT. The secondary objectives were comparisons of events of hypoglycemia, defined as 20 min or more with SG <3.5 mmol/L, and the average percentage of time spent with SG <3.0 mmol/L and in hyperglycemia (SG 10–15 mmol/L and >15 mmol/L) with and without PLGM. The study also evaluated the time spent in hypoglycemia during the day (6:00 A.M. to 10:00 P.M.) and


night (10:00 P.M. to 6:00 A.M.). The percentage time in the glucose range of interest was calculated at each visit by dividing the number of observed CGM readings falling within the respective range by the total number of readings for the time period.

In addition, the safety of the system was determined by evaluating the number of ketosis events (blood ketones >0.6 mmol/L) and glycemic control (HbA<sub>1c</sub>) at the end of 6 months. Using validated questionnaires, the study also evaluated the impact of PLGM on the patient’s quality of life, fear of hypoglycemia, satisfaction and acceptability of the system, and hypoglycemia awareness. A data safety and monitoring board independently reviewed the data arising from the study.

**Statistical Analysis**

A modified intent-to-treat (ITT) approach was used for analysis. The ITT population was defined as all patients who were randomized and had at least one visit (visit four) after randomization. The percentages of time in hypoglycemia and hyperglycemia were calculated for each visit after randomization and were analyzed using likelihood-based, linear mixed-effect model repeated measurement. Models included fixed-effect terms for group, visit, site, baseline time in range, and group by visit interaction. Choice of correlation matrix was based on Akaike information criterion; in all models, the unstructured matrix resulted in the best model fit. Least squares (LS) means, based on the fixed terms in the model,

and differences in LS mean change along with their 95% CIs were calculated. Incidence of severe hypoglycemia and SG-defined hypoglycemic events were analyzed as unadjusted incidence rates based on the Poisson distribution. Ketosis events are presented as percentage of total ketone measurements that were >0.6 mmol/L, and an incidence rate ratio was derived from a negative binomial mixed model analyzing the number of ketosis events with the total number of ketone measurements as the exposure variable. (One participant in the PLGM group on low-carbohydrate diet was excluded from analysis.) Mixed-effect model repeated measurements were conducted using SAS (version 9.4), and all other analyses were conducted

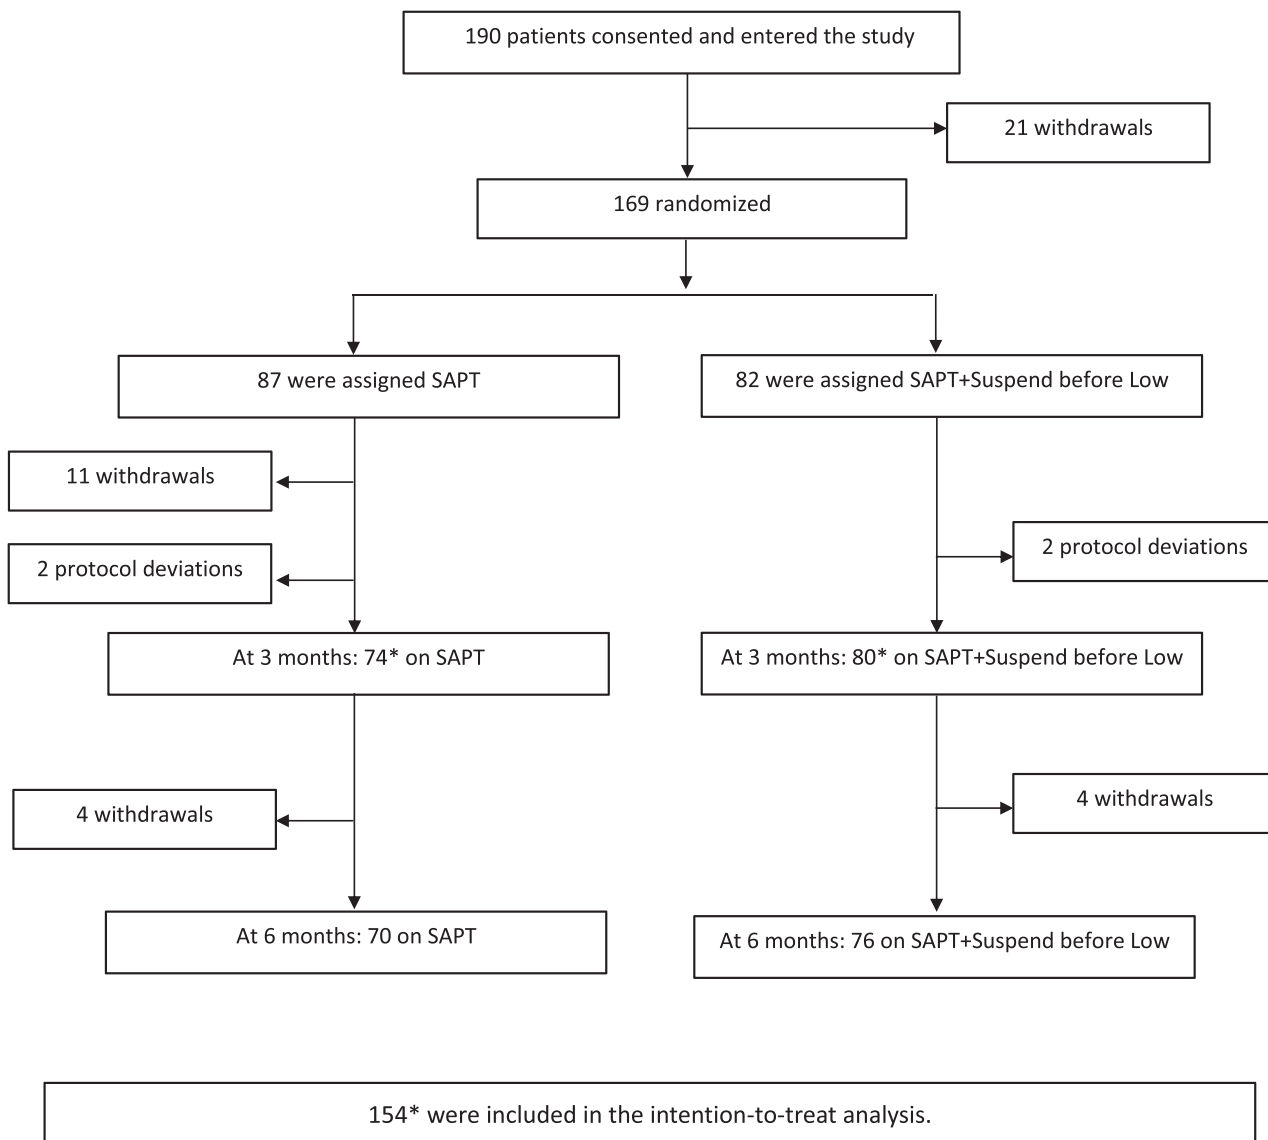

Downloaded from <http://diabetesjournals.org/care/article-pdf/46/12/303/554413/dec17604.pdf> by guest on 07 June 2023

**Figure 1**—The consort diagram for participants in the trial.

using Stata (version 13.0). A  $P$  value  $<0.05$  was considered statistically significant.

## RESULTS

### Study Recruitment and Baseline Characteristics

As illustrated in Fig. 1, 190 participants consented and entered the study. Twenty-one participants withdrew in the run-in period. Eligible participants were randomized with 87 to the control arm and 82 to the intervention arm. Eleven participants withdrew between randomization (visit three) and visit four, with a further eight withdrawals between visit four and end of the study. The reasons for withdrawal were multifactorial. While difficulty in inserting sensors, pain and bleeding at sensor site, sensor life, inaccuracies, and tape reactions were some of the reasons cited by participants, the intensity of the study, the need for increased parental support in younger children, and ability to comply with uploading the devices were reported by the others. Two participants in the intervention arm were excluded due to a protocol deviation (Suspend on low was activated instead of Suspend before low). The baseline CGM data were missing in two participants in the control arm and they were excluded from analysis. The ITT population comprised all participants who were randomized and attended visit four. The data were therefore analyzed in 154 participants (age  $13.2 \pm 2.8$  years, duration of diabetes  $7.1 \pm 3.8$  years,  $HbA_{1c}$   $7.5 \pm 0.8\%$  [mean  $\pm$  SD]): 74 participants in the control arm and 80 participants in the intervention arm.

Table 1 shows the baseline characteristics of the 154 participants. There were no differences in baseline characteristics between the two groups. At baseline, time spent  $<3.5$  mmol/L in the SAPT group was  $3.0 \pm 3.2\%$  and in the PLGM group was  $2.8 \pm 2.9\%$ . All participants had  $>80\%$  sensor use prior to randomization according to the eligibility criteria (SAPT 88% vs. PLGM 83%). The proportion of time with available sensor data was  $72 \pm 0.02\%$  and  $73 \pm 0.02\%$  between baseline and 3 months and  $59 \pm 0.03\%$  and  $63 \pm 0.03\%$  between 4 and 6 months in participants in the control and intervention groups, respectively. Sensor use remained similar in both groups during the duration of the study ( $P = 0.93$ ). Participants on PLGM had an average of 2.35 suspend events per day.

**Table 1—Baseline characteristics of the participants\***

Characteristic	Control (SAPT)	Intervention (PLGM)	Total
<i>n</i>	74	80	154
Age (years)	$13.3 \pm 2.8$	$13.1 \pm 2.8$	$13.2 \pm 2.8$
Males (%)	53	54	53
Duration of diabetes (years)	$6.9 \pm 3.8$	$7.2 \pm 3.7$	$7.1 \pm 3.8$
$HbA_{1c}$ (%)	$7.4 \pm 0.7$	$7.5 \pm 0.8$	$7.5 \pm 0.8$
Duration of pump therapy (years)	$4.5 \pm 2.7$	$4.6 \pm 2.8$	$4.6 \pm 2.7$
BMI**	$21.4 \pm 3.9$	$21.3 \pm 3.5$	$21.3 \pm 3.7$
% time $<3.5$ mmol/L			
Day + night	$3.0 \pm 3.2$	$2.8 \pm 2.9$	$2.5 \pm 2.8$
Day	$2.5 \pm 2.7$	$2.4 \pm 2.7$	$2.5 \pm 2.7$
Night	$3.8 \pm 5.1$	$3.4 \pm 4.2$	$3.3 \pm 4.4$
% time $<3.0$ mmol/L			
Day + night	$1.4 \pm 1.9$	$1.3 \pm 1.7$	$1.1 \pm 1.8$
Day	$1.1 \pm 1.7$	$1.0 \pm 1.5$	$1.1 \pm 1.6$
Night	$2.0 \pm 3.2$	$1.7 \pm 2.7$	$1.8 \pm 3.0$

Values are means  $\pm$  SD. There were no significant differences between the groups ( $P > 0.05$ ).

\*Participants in the ITT analysis. \*\*BMI is the weight in kilograms divided by the square of the height in meters.

### Time Spent in Hypoglycemia

A reduction in time spent in hypoglycemia (SG  $<3.5$  mmol/L) from the commencement of the study was demonstrated in both groups (SAPT 3% to 2.6%,  $P = 0.03$  vs. PLGM 2.8% to 1.4%,  $P < 0.0001$ ) but was greater with PLGM than SAPT during the entire study period (difference in LS means:  $-0.95\%$  [95% CI  $-1.30, -0.61$ ],  $P < 0.0001$ ). The reduction in hypoglycemia with PLGM was persistent across the 6-month study duration. Over the study period, this equated to 37.7 min/day of time  $<3.5$  mmol/L with SAPT and 20 min/day with PLGM. A similar effect was also noted in time spent with SG  $<3$  mmol/L (SAPT 1.4% to 1.2%,  $P = 0.04$  vs. PLGM 1.3% to 0.6%,  $P < 0.0001$ ), with a greater reduction with PLGM than SAPT (difference in LS means:  $-0.44\%$  [ $-0.64, -0.24$ ],  $P < 0.0001$ ). This corresponds to 17.6 min/day of time  $<3$  mmol/L on SAPT and 9 min/day on PLGM (Fig. 2). SAPT alone was not associated with a statistically significant reduction in hypoglycemia during daytime (2.5% to 2.3%; difference in LS means: 0.23 [ $-0.48, 0.02$ ],  $P = 0.07$ ), although it was accompanied by a small reduction in nocturnal hypoglycemia (3.8% to 3.3%; difference in LS means:  $-0.45\%$  [ $-0.88, -0.02$ ],  $P = 0.04$ ). In contrast, PLGM use resulted in hypoglycemia reduction both during day and night (day 2.4% to 1.3%; difference in LS means:  $-1.09\%$  [ $-1.33, -0.85$ ],  $P < 0.001$ ; vs. night 3.4% to 1.6%; difference in LS means:  $-1.96\%$  [ $-2.37, -1.54$ ],  $P < 0.0001$ ), with a difference in LS means

of 1.51% (0.92, 2.10;  $P < 0.001$ ) between both groups.

### Hypoglycemic Events


Both groups had a similar number of sensor-defined hypoglycemic events (SG  $<3.5$  mmol/L for  $>20$  min) during the run-in period (SAPT vs. PLGM, events/patient-year: 232 vs. 245 [95% CI 217, 248 vs. 230, 261],  $P = 0.245$ ). However, at the end of the study, the PLGM group had fewer hypoglycemic events compared with those on SAPT (SAPT vs. PLGM, events/patient-year: 227 vs. 139 [95% CI 221, 234 vs. 134, 143],  $P < 0.001$ ). There were no episodes of severe hypoglycemia in either group during the 6-month study period.

### Impaired Awareness of Hypoglycemia

At baseline, there were 90 participants  $\geq 12$  years of age. Of these, impaired awareness of hypoglycemia (IAH; Clarke score  $\geq 4$ ) was present in 17% at baseline ( $n = 15$ ), with a similar number in each group (SAPT 16% vs. PLGM 18%). At the end of 6 months, the prevalence of IAH in the SAPT group was 13% and 4% in the PLGM group. A mixed-effects logistic regression did not demonstrate a significant effect of intervention group (odds ratio 0.25 [0.03, 1.84],  $P = 0.17$ ; reference category was SAPT). There was no effect of PLGM on the mean Clarke scores in the aware and IAH group (difference in LS means:  $-0.04$  [ $-0.52, 0.43$ ],  $P = 0.86$ ).

### Safety and Adverse Events

An increase in time spent in SG 10–15 mmol/L was seen with SAPT and PLGM (SAPT 27% to 31%,  $P < 0.0001$  vs.

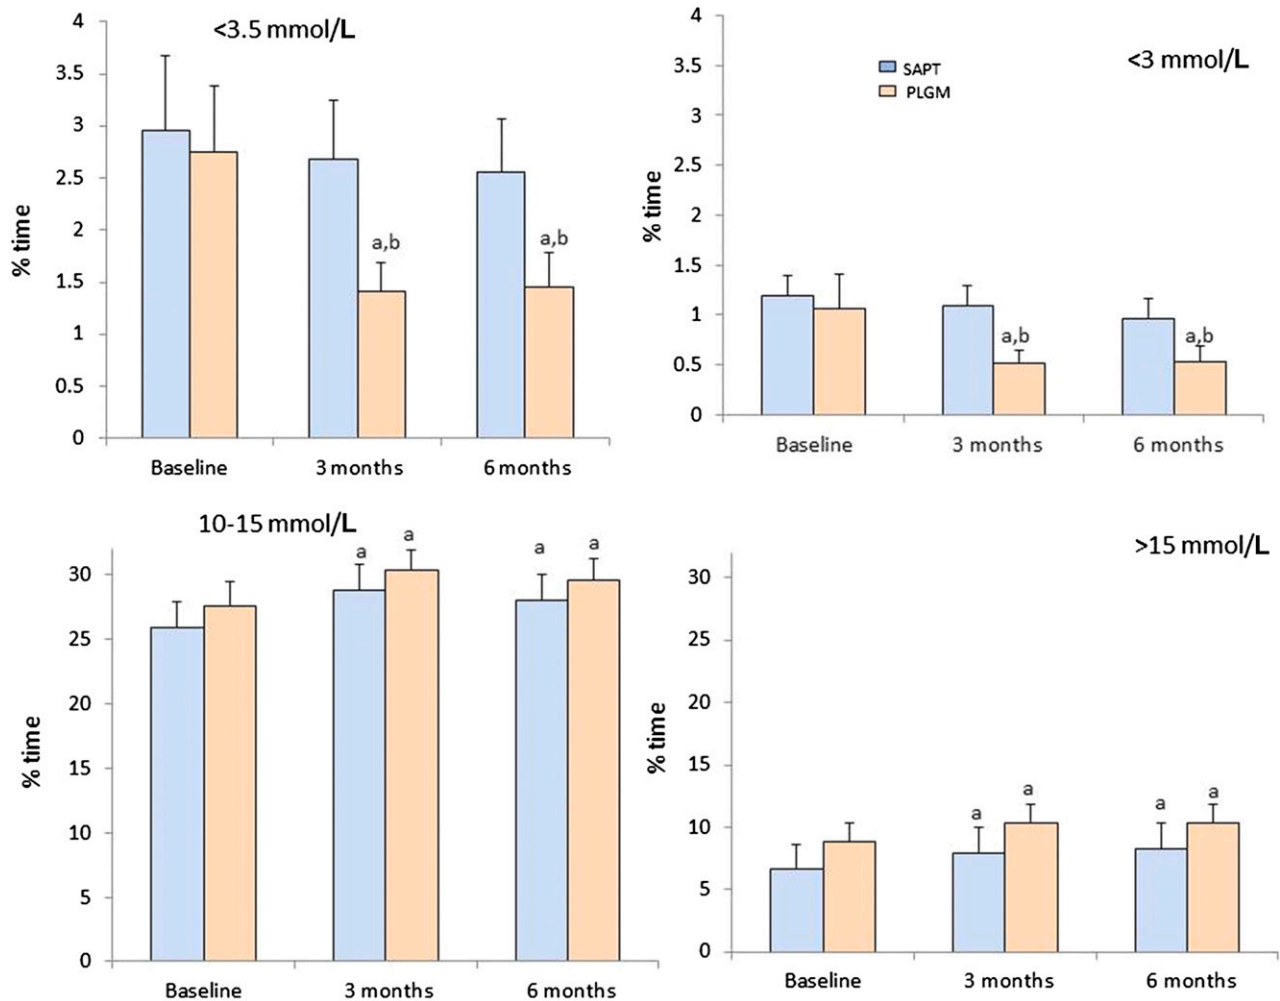

**Figure 2**—The time in hypoglycemia (SG <3.5 mmol/L and <3 mmol/L) and hyperglycemia (SG 10–15 mmol/L and >15 mmol/L). a, change from baseline,  $P < 0.005$ ; b, difference between groups,  $P < 0.005$ .

PLGM 29% to 31%,  $P < 0.0001$ ). However, there was no effect of the intervention on time spent in 10–15 mmol/L at the end of the study (difference in LS means: 0.47 [95% CI  $-1.1, 2.1$ ],  $P = 0.56$ ). Similarly, an increase in time >15 mmol/L was seen in both groups (SAPT 7% to 10%,  $P < 0.0001$  vs. PLGM 9% to 10%,  $P < 0.0001$ ), although there was no difference between the two groups at the end of the study (difference in LS means: 0.52 [  $-0.73, 1.78$ ],  $P = 0.40$ ). The mean SG was 9.3 mmol/L (9.1, 9.5) and 9.8 mmol/L (9.5, 10) in the control and intervention groups, respectively ( $P < 0.005$ ). However, the HbA<sub>1c</sub> level from randomization to study end was unchanged in both study groups (SAPT  $7.4 \pm 0.7\%$  to  $7.6 \pm 1.0\%$ ,  $P = 0.20$  vs. PLGM  $7.5 \pm 0.8\%$  to  $7.8 \pm 0.8\%$ ,  $P = 0.008$ ), with the difference in LS means of 0.09 ( $-0.10, 0.27$ ;  $P = 0.35$ ). There was no difference in the ketosis events (>0.6 mmol/L) between

the two groups (SAPT 2.2% vs. PLGM 2.6%; incidence rate ratio 0.96 [0.52, 1.76],  $P = 0.89$ ). Apart from one episode of diabetic ketoacidosis due to pump failure and poor management in the PLGM group, there were no severe adverse events in the study period.

#### Quality of Life and Fear of Hypoglycemia

At the end of the study, participants and their parents reported no change in quality of life measures in either group. Similarly, there was no difference in fear of hypoglycemia between the two groups. Table 2 provides the scores of the participants and their parents in both groups.

#### CONCLUSIONS

This study highlights an almost twofold reduction in hypoglycemia exposure in children and adolescents with type 1

diabetes using PLGM during a 6-month, multicenter, randomized controlled home trial. These results support the findings of the in-clinic studies that used the investigational PLGM system (4–6) and the short-term observational studies and trials that used the MiniMed 640G pump with the SmartGuard function in children and adults (7–12). In our study, both groups demonstrated a reduction in hypoglycemia, although the magnitude of reduction was greater with PLGM. The use of SAPT did not significantly reduce the time spent in hypoglycemia during the day but showed a mild reduction at night. In contrast, PLGM was associated with reduced day and nighttime hypoglycemia, with greater reduction at night. Children and adolescents spent approximately half the time in hypoglycemia with fewer hypoglycemic events with PLGM as compared with SAPT alone. The lower hypoglycemia exposure was consistent in subgroups of participants

**Table 2—IAH, quality of life, fear of hypoglycemia, and CGM satisfaction in participants and parents in the trial**

Questionnaire	Component	Respondent	Baseline		6 months		P
			SAPT	PLGM	SAPT	PLGM	
Time <3 mmol/L							
IAH (n)	n	Child*	7	8	6	2	0.17
	Score		2.0 ± 1.7	1.8 ± 1.5	1.7 ± 1.5	1.7 ± 1.2	0.86
Quality of life	VAS	Child*	81.8 ± 14.3	85.4 ± 9.3	85.7 ± 14.0	81.5 ± 17.2	0.69
		Parent	84.8 ± 11.9	85.2 ± 11.4	84.2 ± 13.5	85.5 ± 11.9	0.61
	Index	Child*	0.86 ± 0.11	0.90 ± 0.13	0.83 ± 0.25	0.85 ± 0.24	0.45
		Parent	0.84 ± 0.17	0.87 ± 0.14	0.81 ± 0.22	0.90 ± 0.11	0.50
Pediatric quality of life	Total	8–12 years	72.5 ± 13.3	72.7 ± 11.4	71.0 ± 13.2	71.9 ± 11.5	0.65
		>12 years	68.1 ± 13.2	68.6 ± 11.0	69.7 ± 15.3	68.3 ± 11.7	0.55
		Parent	65.1 ± 13.9	68.3 ± 12.1	63.2 ± 13.8	66.2 ± 12.1	0.45
Fear of hypoglycemia	Total	Child*	35.3 ± 13.5	34.5 ± 14.4	32.6 ± 11.9	31.8 ± 14.8	0.40
		Parent	46.7 ± 15.1	44.8 ± 16.0	44.9 ± 14.5	42.1 ± 14.7	0.29
	Behavior	Child*	18.9 ± 5.2	17.0 ± 6.4	19.2 ± 6.0	16.8 ± 6.5	0.82
		Parent	23.1 ± 6.6	21.9 ± 7.2	23.4 ± 7.0	20.8 ± 7.0	0.20
	Worry	Child*	16.3 ± 10.8	17.5 ± 10.3	13.4 ± 8.0	15.0 ± 10.5	0.16
		Parent	23.6 ± 11.8	22.9 ± 11.3	21.5 ± 10.3	21.3 ± 10.2	0.53
CGM satisfaction	Total	Child*	3.5 ± 0.3	3.6 ± 0.3	3.4 ± 0.4	3.5 ± 0.4	0.46
		Parent	3.6 ± 0.3	3.7 ± 0.3	3.5 ± 0.4	3.5 ± 0.3	0.12

IAH is expressed in numbers (n) and score; quality of life, fear of hypoglycemia, and CGM satisfaction are expressed as scores.  $P < 0.05$ : significant, derived from mixed models including data from 3 months and 6 months adjusting for baseline. VAS, visual analogue scale. \*Self-reported by children >12 years of age.

irrespective of the age, duration of diabetes, HbA<sub>1c</sub> level, and hypoglycemia awareness status. In our study, the baseline time in hypoglycemia was relatively low (38 min/day with SG <3.5 mmol/L or 18 min/day with SG <3 mmol/L); this contrasts with older studies but is similar to other recent studies with 73 min/day with SG <3.9 mmol/L in a German study (7) and 45 and 29 min/day, respectively, with SG <3.6 and <3.3 mmol/L in a study from Slovenia and Israel (12). These groups also showed a significant reduction in hypoglycemia by at least 50%. This does highlight that hypoglycemia was reduced in contemporary samples, perhaps with improved modalities of treatment.

The decline in hypoglycemia exposure was not associated with an increase in hyperglycemia with PLGM as compared with SAPT. Although the time spent between 10–15 mmol/L and >15 mmol/L increased from baseline in both groups, there was no evidence for a difference between the control and intervention arm in spite of automated insulin suspends with PLGM. It is reassuring to note that insulin suspension by itself may not be the cause of the increase in hyperglycemia, and the observation that an increase in SG >10 mmol/L was noted in both groups could possibly be due

to carbohydrate consumption by the participants to prevent hypoglycemia when CGM readings alerted them to falling glucose levels. In contrast to the previously conducted short-term studies, the 6-month study duration provided us with the opportunity to follow the glycemic outcomes. Although there was an increase in HbA<sub>1c</sub> from baseline with PLGM, there was no difference in the HbA<sub>1c</sub> between the two groups at the end of 6 months. The safety of the system was further established with a similar proportion of ketosis in both groups. This is in accordance with previous studies that, although using a different predictive algorithm (Kalman filter predictive model), demonstrated a reduction in overnight hypoglycemia with predictive suspends without conferring an increased risk of morning ketosis (20,21). This further reinforces the efficacy of the system in reducing the time spent in hypoglycemia without deterioration of glycemic control.

The 6-month study duration further helped us to explore the impact of this technology on various psychosocial parameters in both children and their caregivers. Most participants were sensor naïve at the commencement of the study, and both groups used the same pump and sensors with PLGM enabled in the intervention group. The need of an

additional sensor site, troubleshooting sensor problems, and coping with alarms and alerts with additional pump suspends and resumptions in the intervention group could potentially increase the burden of the disease. Hence, it is reassuring to note that there was no deterioration in the quality of life in both groups during the study. Furthermore, the expected reduction in fear of hypoglycemia was not evidenced in our cohort. There was no difference between the control and intervention groups at the end of the study in both children and their caregivers. This could be as PLGM does not completely abolish hypoglycemia, although it reduces the number of hypoglycemic events.

The SmartGuard option with the Suspend on low and Suspend before low functions empower the user to individualize diabetes management. A CareLink review of the MiniMed 640G pump demonstrated that at least 99% of all users used one or both suspend functions and 59% used Suspend before low exclusively (9). The threshold level for pump suspend can be individualized by the user for different times of the day. A higher threshold has a greater chance to abort an impending hypoglycemic event, albeit with an increase in the number of alarms, suspensions, hyperglycemia post-resumption, and possible patient fatigue.

On the contrary, a lower threshold could avoid the multiple suspensions but may not eliminate the risk of hypoglycemia. In recent studies, either the low limit was chosen by the participant (10) or the hypoglycemia threshold (3.9 mmol/L) was set for the whole study (7). In our study, we set the lower limit at 3.4 mmol/L (pump suspend if SG  $\leq$  4.5 mmol/L in 30 min). We used this low limit as a result of our experience in the in-clinic studies (4,5) and the PILGRIM study (6). We maintained the same threshold throughout the study to provide uniformity to the entire intervention group and to establish a threshold that would not be associated with clinically significant post-suspend hyperglycemia. However, in real-life, these thresholds can be altered and individualized depending on the glycemic excursions related to food and exercise in day-to-day life.

The reduction in the duration of hypoglycemia and hypoglycemic episodes was accompanied by a nonstatistically significant trend toward reduced prevalence of IAH with the use of PLGM. Although this result did not reach statistical significance, this outcome was only available for a smaller subpopulation of the sample. The observed, albeit nonsignificant, trend suggests that the reduced prevalence of IAH is potentially a clinically important secondary outcome that requires further study. Therapeutic options for patients with IAH remain limited and challenging, and although some individuals may gain benefit from structured education, the use of CGM, and SAPT with low glucose suspension, many do not respond to these approaches (22). Hypoglycemia avoidance is the basis of restoring awareness in patients with IAH (23,24), and systems like PLGM, by almost eliminating hypoglycemia, have the potential to improve awareness in this high-risk group and provide a valuable addition to the current armamentarium of available therapies.

Sustained frequent use of CGM is challenging in children and adolescents compared with adults, with sensor uptake higher in adults than among children. The Star 3 trial continuation phase reported a mean sensor wear time of 61% among adults and 45% among pediatric subjects (25). Similarly, the JDRF-CGM follow-up trial reported sensor wear of 6.5, 3.3, and 3.7 days/week in the 6th month in participants >25 years, 15–24 years,

and 8–14 years, respectively (26). In our study, time commitment, technical challenges, sensor alerts, sensor efficacy, sensor life, and skin irritation were described as some of the barriers identified through open-ended questionnaires (27). These challenges are potentially compounded in the adolescent age-group, a physical and emotional growth phase associated with risk taking and vulnerability (28). Hence, it is vital to address these issues with participants and their families to provide them with education and support to overcome and troubleshoot these issues.

This study is the first randomized controlled home trial and provides high-quality evidence of the efficacy and safety of the PLGM system in the prevention of hypoglycemia in real-life situations. The strength of our study is in its ability to provide this clinical insight about the use of PLGM in free-living conditions. A limitation of our study is that the important clinical observation of reduced prevalence of IAH in participants on PLGM did not reach statistical significance. We were also unable to corroborate it with improved counterregulatory hormones as originally planned in our study design, as the prevalence of IAH in this cohort was 17% as compared with the expected 25% of patients (29), which affected recruitment for this outcome. Hence, the small sample size of this high-risk group provides only observational inferences.

To conclude, PLGM reduced hypoglycemia exposure without compromising glycemic control or quality of life in children and adolescents with type 1 diabetes and thereby is an important technological device to reduce hypoglycemia in their day-to-day lives.

**Funding.** The study was funded by JDRF Australia (JDRF 17-2011-664), the recipient of the Australian Research Council Special Research Initiative in Type 1 Juvenile Diabetes. The research was also supported by Medtronic through the provision of insulin pumps, sensors, and transmitters for the study. M.B.A. was supported by a JDRF mentored clinical research fellowship.

**Duality of Interest.** No potential conflicts of interest relevant to this article were reported.

**Author Contributions.** M.B.A. conducted and coordinated the studies, collected data, and wrote the manuscript. J.A.N. contributed to the design of the study, conducted and coordinated the studies, and reviewed the manuscript. G.J.S. collected data, conducted the analyses, and provided statistical input. J.M.F., B.R.K., G.R.A., F.J.C., E.A.D., and T.W.J. contributed to the design of

the study, supervised the study at each site, and reviewed the manuscript. T.W.J. is the guarantor of this work and, as such, had full access to all the data in the study and takes responsibility for the integrity of the data and the accuracy of the data analysis.

## References

- Bergenstal RM, Tamborlane WV, Ahmann A, et al.; STAR 3 Study Group. Effectiveness of sensor-augmented insulin-pump therapy in type 1 diabetes. *N Engl J Med* 2010;363:311–320
- Bergenstal RM, Klonoff DC, Garg SK, et al.; ASPIRE In-Home Study Group. Threshold-based insulin-pump interruption for reduction of hypoglycemia. *N Engl J Med* 2013;369:224–232
- Ly TT, Nicholas JA, Retterath A, Lim EM, Davis EA, Jones TW. Effect of sensor-augmented insulin pump therapy and automated insulin suspension vs standard insulin pump therapy on hypoglycemia in patients with type 1 diabetes: a randomized clinical trial. *JAMA* 2013;310:1240–1247
- Abraham MB, Davey R, O'Grady MJ, et al. Effectiveness of a predictive algorithm in the prevention of exercise-induced hypoglycemia in type 1 diabetes. *Diabetes Technol Ther* 2016;18:543–550
- Abraham MB, de Bock M, Paramalingam N, et al. Prevention of insulin-induced hypoglycemia in type 1 diabetes with predictive low glucose management system. *Diabetes Technol Ther* 2016;18:436–443
- Danne T, Tzioli C, Kordonouri O, et al. The PILGRIM Study: in silico modeling of a predictive low glucose management system and feasibility in youth with type 1 diabetes during exercise. *Diabetes Technol Ther* 2014;16:338–347
- Biester T, Kordonouri O, Holder M, et al. "Let the algorithm do the work": reduction of hypoglycemia using sensor-augmented pump therapy with predictive insulin suspension (SmartGuard) in pediatric type 1 diabetes patients. *Diabetes Technol Ther* 2017;19:173–182
- Scaramuzza AE, Arnaldi C, Cherubini V, et al. Use of the predictive low glucose management (PLGM) algorithm in Italian adolescents with type 1 diabetes: CareLink™ data download in a real-world setting. *Acta Diabetol* 2017;54:317–319
- Zhong A, Choudhary P, McMahon C, et al. Effectiveness of automated insulin management features of the MiniMed® 640G sensor-augmented insulin pump. *Diabetes Technol Ther* 2016;18:657–663
- Choudhary P, Olsen BS, Conget I, Welsh JB, Vorrink L, Shin JJ. Hypoglycemia prevention and user acceptance of an insulin pump system with predictive low glucose management. *Diabetes Technol Ther* 2016;18:288–291
- Villafuerte Quispe B, Martin Frias M, Roldan Martin MB, Yelmo Valverde R, Alvarez Gomez MA, Barrio Castellanos R. Effectiveness of MiniMed 640G with SmartGuard® System for prevention of hypoglycemia in pediatric patients with type 1 diabetes mellitus. *Endocrinol Diabetes Nutr* 2017;64:198–203
- Battelino T, Nimri R, Dovc K, Phillip M, Bratina N. Prevention of hypoglycemia with predictive low glucose insulin suspension in children with type 1 diabetes: a randomized controlled trial. *Diabetes Care* 2017;40:764–770

13. Bulsara MK, Holman CD, Davis EA, Jones TW. The impact of a decade of changing treatment on rates of severe hypoglycemia in a population-based cohort of children with type 1 diabetes. *Diabetes Care* 2004;27:2293–2298
14. Abraham MB, Nicholas JA, Ly TT, et al. Safety and efficacy of the predictive low glucose management system in the prevention of hypoglycaemia: protocol for randomised controlled home trial to evaluate the Suspend before low function. *BMJ Open* 2016;6:e011589
15. Saghaei M. An overview of randomization and minimization programs for randomized clinical trials. *J Med Signals Sens* 2011;1:55–61
16. Clarke WL, Cox DJ, Gonder-Frederick LA, Julian D, Schlundt D, Polonsky W. Reduced awareness of hypoglycemia in adults with IDDM. A prospective study of hypoglycemic frequency and associated symptoms. *Diabetes Care* 1995;18:517–522
17. Varni JW, Curtis BH, Abetz LN, Lasch KE, Piault EC, Zeytoonjian AA. Content validity of the PedsQL™ 3.2 Diabetes Module in newly diagnosed patients with type 1 diabetes mellitus ages 8–45. *Qual Life Res* 2013;22:2169–2181
18. Cox DJ, Irvine A, Gonder-Frederick L, Nowacek G, Butterfield J. Fear of hypoglycemia: quantification, validation, and utilization. *Diabetes Care* 1987;10:617–621
19. Juvenile Diabetes Research Foundation Continuous Glucose Monitoring Study Group. Validation of measures of satisfaction with and impact of continuous and conventional glucose monitoring. *Diabetes Technol Ther* 2010;12:679–684
20. Maahs DM, Calhoun P, Buckingham BA, et al.; In Home Closed Loop Study Group. A randomized trial of a home system to reduce nocturnal hypoglycemia in type 1 diabetes. *Diabetes Care* 2014;37:1885–1891
21. Buckingham BA, Cameron F, Calhoun P, et al. Outpatient safety assessment of an in-home predictive low-glucose suspend system with type 1 diabetes subjects at elevated risk of nocturnal hypoglycemia. *Diabetes Technol Ther* 2013;15:622–627
22. Ly TT, Maahs DM, Rewers A, Dunger D, Oduwole A, Jones TW; International Society for Pediatric and Adolescent Diabetes. ISPAD Clinical Practice Consensus Guidelines 2014. Assessment and management of hypoglycemia in children and adolescents with diabetes. *Pediatr Diabetes* 2014;15(Suppl. 20):180–192
23. Cranston I, Lomas J, Maran A, Macdonald I, Amiel SA. Restoration of hypoglycaemia awareness in patients with long-duration insulin-dependent diabetes. *Lancet* 1994;344:283–287
24. Fanelli CG, Epifano L, Rambotti AM, et al. Meticulous prevention of hypoglycemia normalizes the glycemic thresholds and magnitude of most of neuroendocrine responses to, symptoms of, and cognitive function during hypoglycemia in intensively treated patients with short-term IDDM. *Diabetes* 1993;42:1683–1689
25. Bergenstal RM, Tamborlane WV, Ahmann A, et al.; STAR 3 Study Group. Sensor-augmented pump therapy for A1C reduction (STAR 3) study: results from the 6-month continuation phase. *Diabetes Care* 2011;34:2403–2405
26. Juvenile Diabetes Research Foundation Continuous Glucose Monitoring Study Group. Effectiveness of continuous glucose monitoring in a clinical care environment: evidence from the Juvenile Diabetes Research Foundation continuous glucose monitoring (JDRF-CGM) trial. *Diabetes Care* 2010;33:17–22
27. Nicholas JA, Gill FJ, Elliott L, et al. Sensor-augmented pump therapy in the management of type 1 diabetes: lived experiences of children, adolescents and parents. *Australian Diabetes Educator* 2017;20:30–38
28. Jaser SS, Yates H, Dumser S, Whittemore R. Risky business: risk behaviors in adolescents with type 1 diabetes. *Diabetes Educ* 2011;37:756–764
29. Ly TT, Gallego PH, Davis EA, Jones TW. Impaired awareness of hypoglycemia in a population-based sample of children and adolescents with type 1 diabetes. *Diabetes Care* 2009;32:1802–1806